

Sample Name : DYKDDDDK Peptide
 Cat No. : RP10586 Lot No.: PE2431709

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

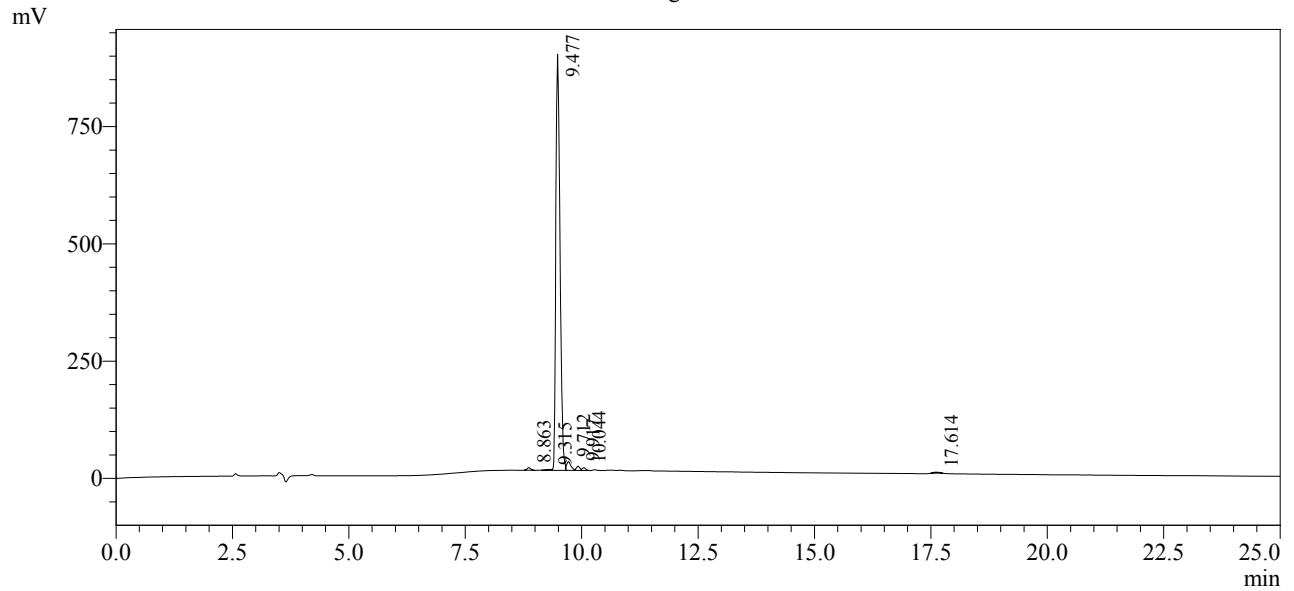

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.863	28950	5533	0.501
2	9.315	13718	1917	0.238
3	9.477	5515524	886783	95.498
4	9.712	119948	18666	2.077
5	9.917	47778	9102	0.827
6	10.044	29574	5880	0.512
7	17.614	20070	2317	0.347
Total		5775561	930199	100.000