

Sample Name :SV40 large T antigen NLS  
 Cat No. :RP20414  
 Lot No. :E5573019J  
 Time Processed :8:50:17  
 Month-Day-Year Processed :10/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010507

<Chromatogram>

mV

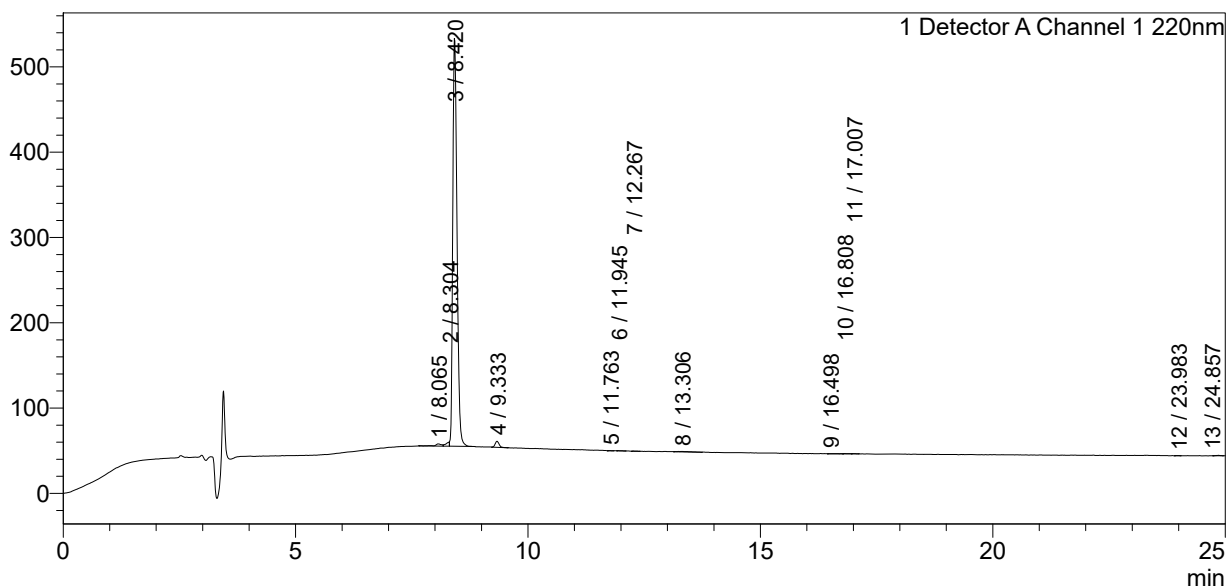

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.065	23702	2602	0.754
2	8.304	25042	4712	0.797
3	8.420	3030728	478002	96.399
4	9.333	42268	7223	1.344
5	11.763	1019	238	0.032
6	11.945	1083	201	0.034
7	12.267	1688	284	0.054
8	13.306	8721	441	0.277
9	16.498	2188	212	0.070
10	16.808	2139	312	0.068
11	17.007	1479	301	0.047
12	23.983	1190	260	0.038
13	24.857	2692	487	0.086
Total		3143939	495276	100.000