

Sample Name :Secretin, human
 Cat No. :RP10249
 Lot No. :E9332821B
 Time Processed :4:17:11
 Month-Day-Year Processed :02/07/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

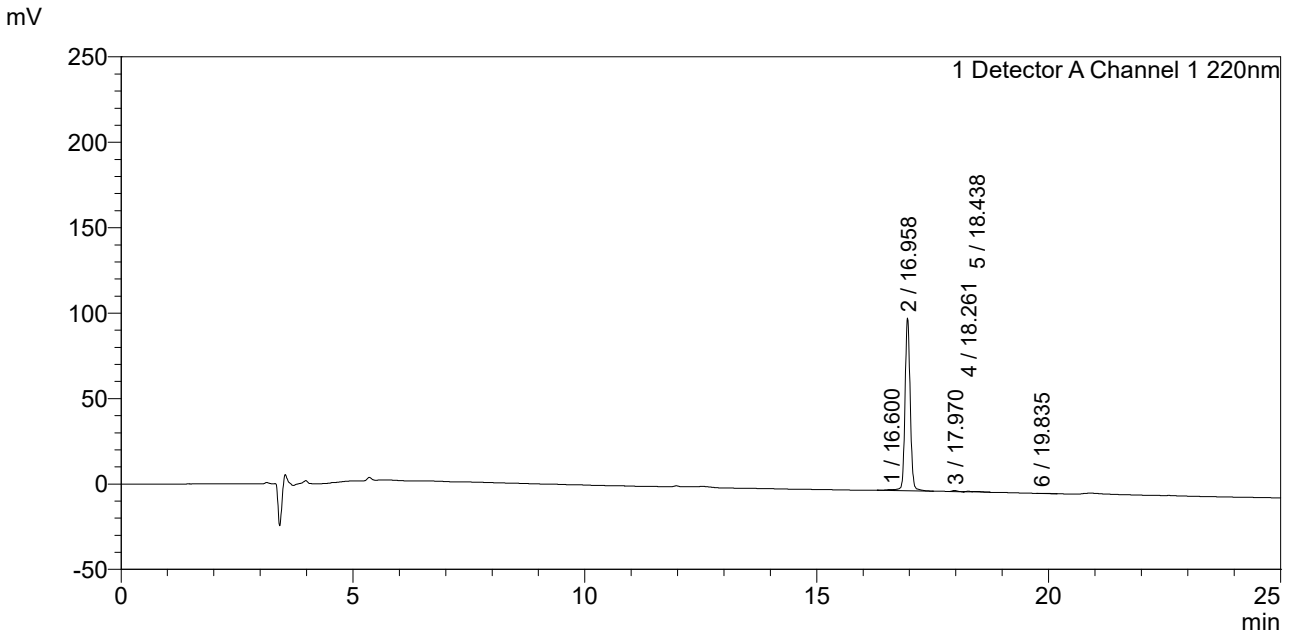

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.600	6192	576	0.767
2	16.958	787931	101088	97.572
3	17.970	4686	652	0.580
4	18.261	2407	323	0.298
5	18.438	4469	367	0.553
6	19.835	1853	120	0.229
Total		807536	103125	100.000