

Sample Name : Transdermal Peptide  
 Cat No. : RP20404  
 Lot No. : E5955120C  
 Time Processed : 10:17:52  
 Month-Day-Year Processed : 04/04/20

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
5.00	Pumps	Solvent B Conc.	0
20.00	Pumps	Solvent B Conc.	30
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	0
40.00	Pumps	Solvent B Conc.	0
40.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ17010508

### <Chromatogram>

mV

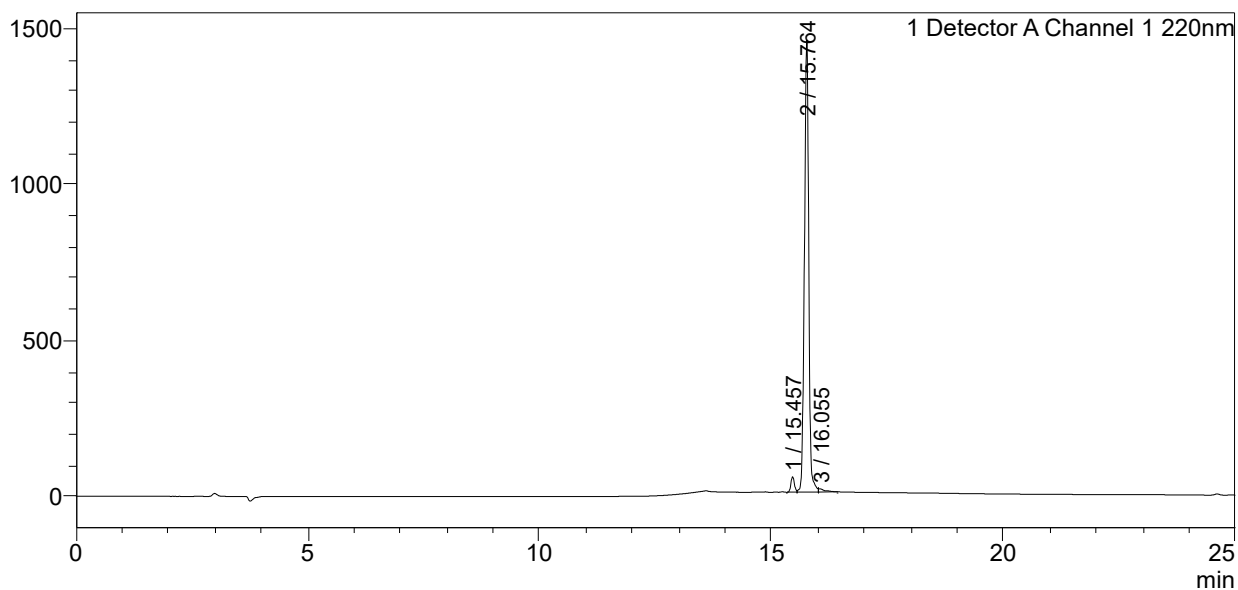

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.457	260340	49244	2.669
2	15.764	9409900	1450951	96.458
3	16.055	85224	9576	0.874
Total		9755465	1509772	100.000