

Sample Name :DYKDDDDKpeptide
 Cat No. :RP10586
 Lot No. :PE8151902
 Time Processed :10:15:41
 Month-Day-Year Processed :03/02/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

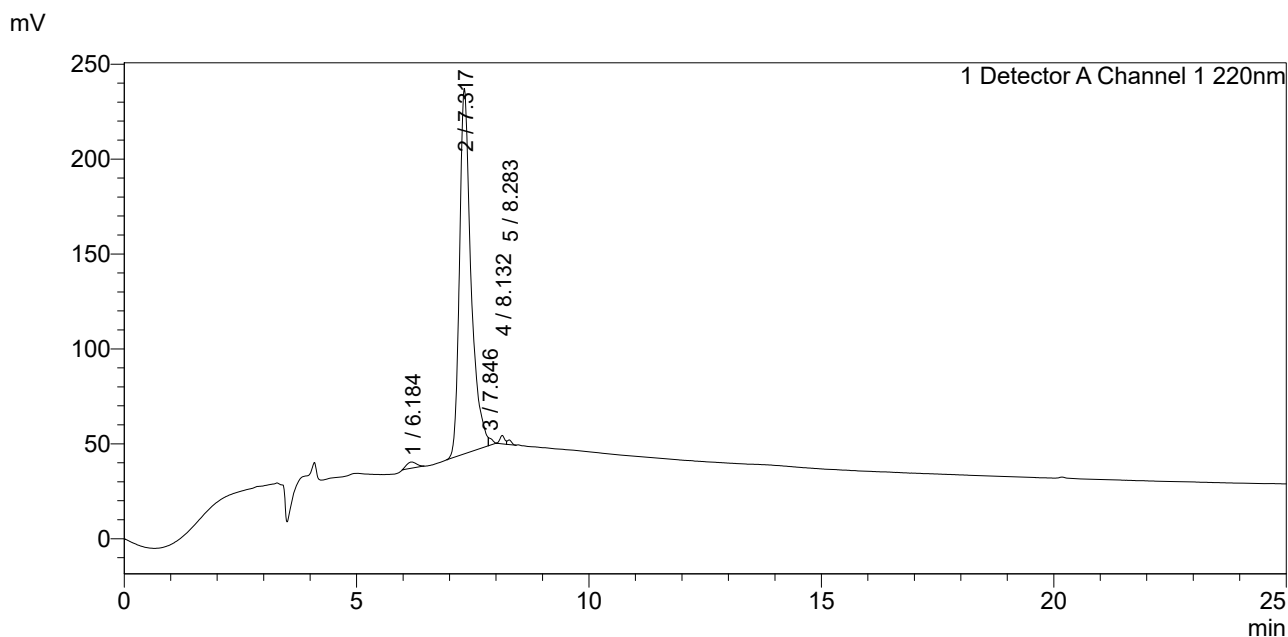

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.184	48503	3248	1.416
2	7.317	3307341	192525	96.577
3	7.846	22383	4124	0.654
4	8.132	31342	4432	0.915
5	8.283	14995	2426	0.438
Total		3424565	206755	100.000