

Sample Name :C-Peptide (3-33), human  
 Cat No.: RP11116  
 Lot No.: E8770420D  
 Time Processed :20:56:14  
 Month-Day-Year Processed :04/03/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

| Time  | Module     | Command         | Value |
|-------|------------|-----------------|-------|
| 0.01  | Pumps      | Solvent B Conc. | 15    |
| 25.00 | Pumps      | Solvent B Conc. | 75    |
| 25.01 | Pumps      | Solvent B Conc. | 95    |
| 31.00 | Pumps      | Solvent B Conc. | 95    |
| 31.01 | Pumps      | Solvent B Conc. | 15    |
| 40.00 | Pumps      | Solvent B Conc. | 15    |
| 40.01 | Controller | Stop            |       |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

### <Chromatogram>

mV

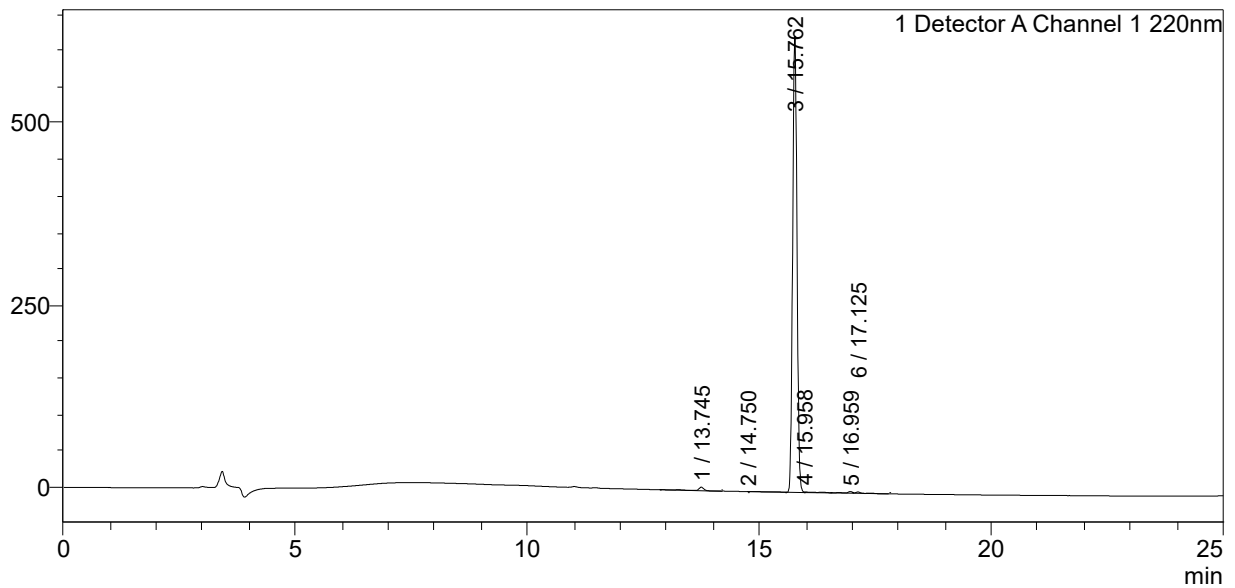

### <Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area    | Height | Area%   |
|-------|-----------|---------|--------|---------|
| 1     | 13.745    | 41086   | 4904   | 0.979   |
| 2     | 14.750    | 1075    | -3     | 0.026   |
| 3     | 15.762    | 4091747 | 626372 | 97.502  |
| 4     | 15.958    | 20809   | 1068   | 0.496   |
| 5     | 16.959    | 22886   | 2466   | 0.545   |
| 6     | 17.125    | 18979   | 1879   | 0.452   |
| Total |           | 4196583 | 636687 | 100.000 |