

Sample Name :CRF, human, rat  
Cat No.: RP10982  
Lot No.: PE6051812  
Time Processed:19:10:20  
Month-Day-Year Processed:12/06/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
Total Flow:1 ml/min  
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

### <Chromatogram>

mV

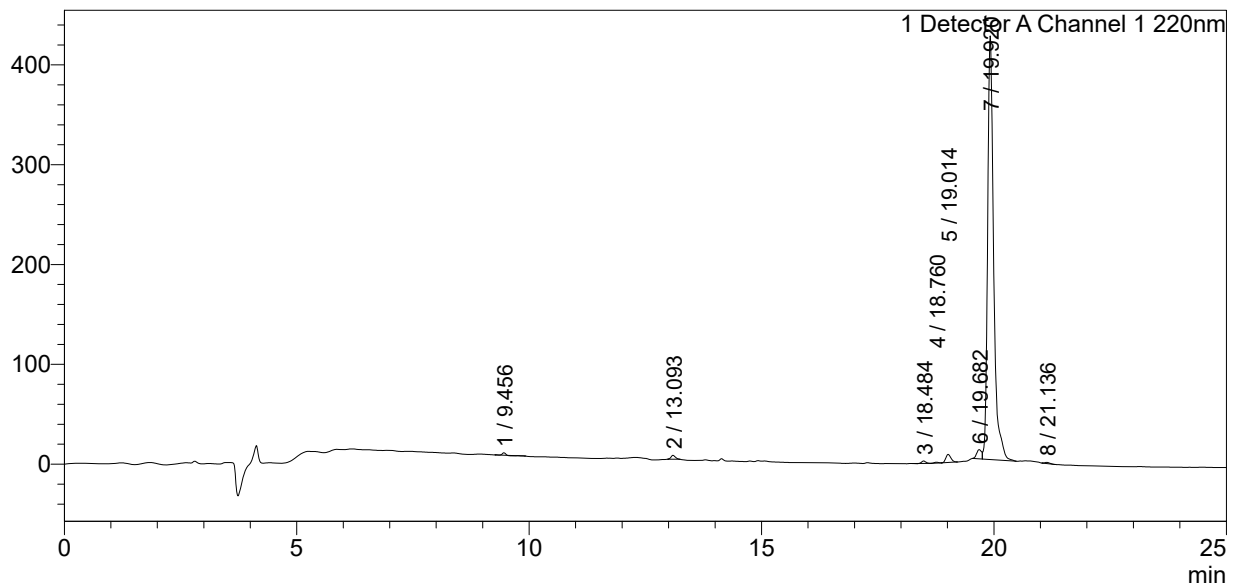

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.456	9098	2423	0.227
2	13.093	24456	3877	0.610
3	18.484	13264	2391	0.331
4	18.760	5648	864	0.141
5	19.014	61854	8102	1.542
6	19.682	67959	9143	1.694
7	19.920	3821339	424323	95.241
8	21.136	8648	1189	0.216
Total		4012265	452311	100.000