


Mass Spectrum

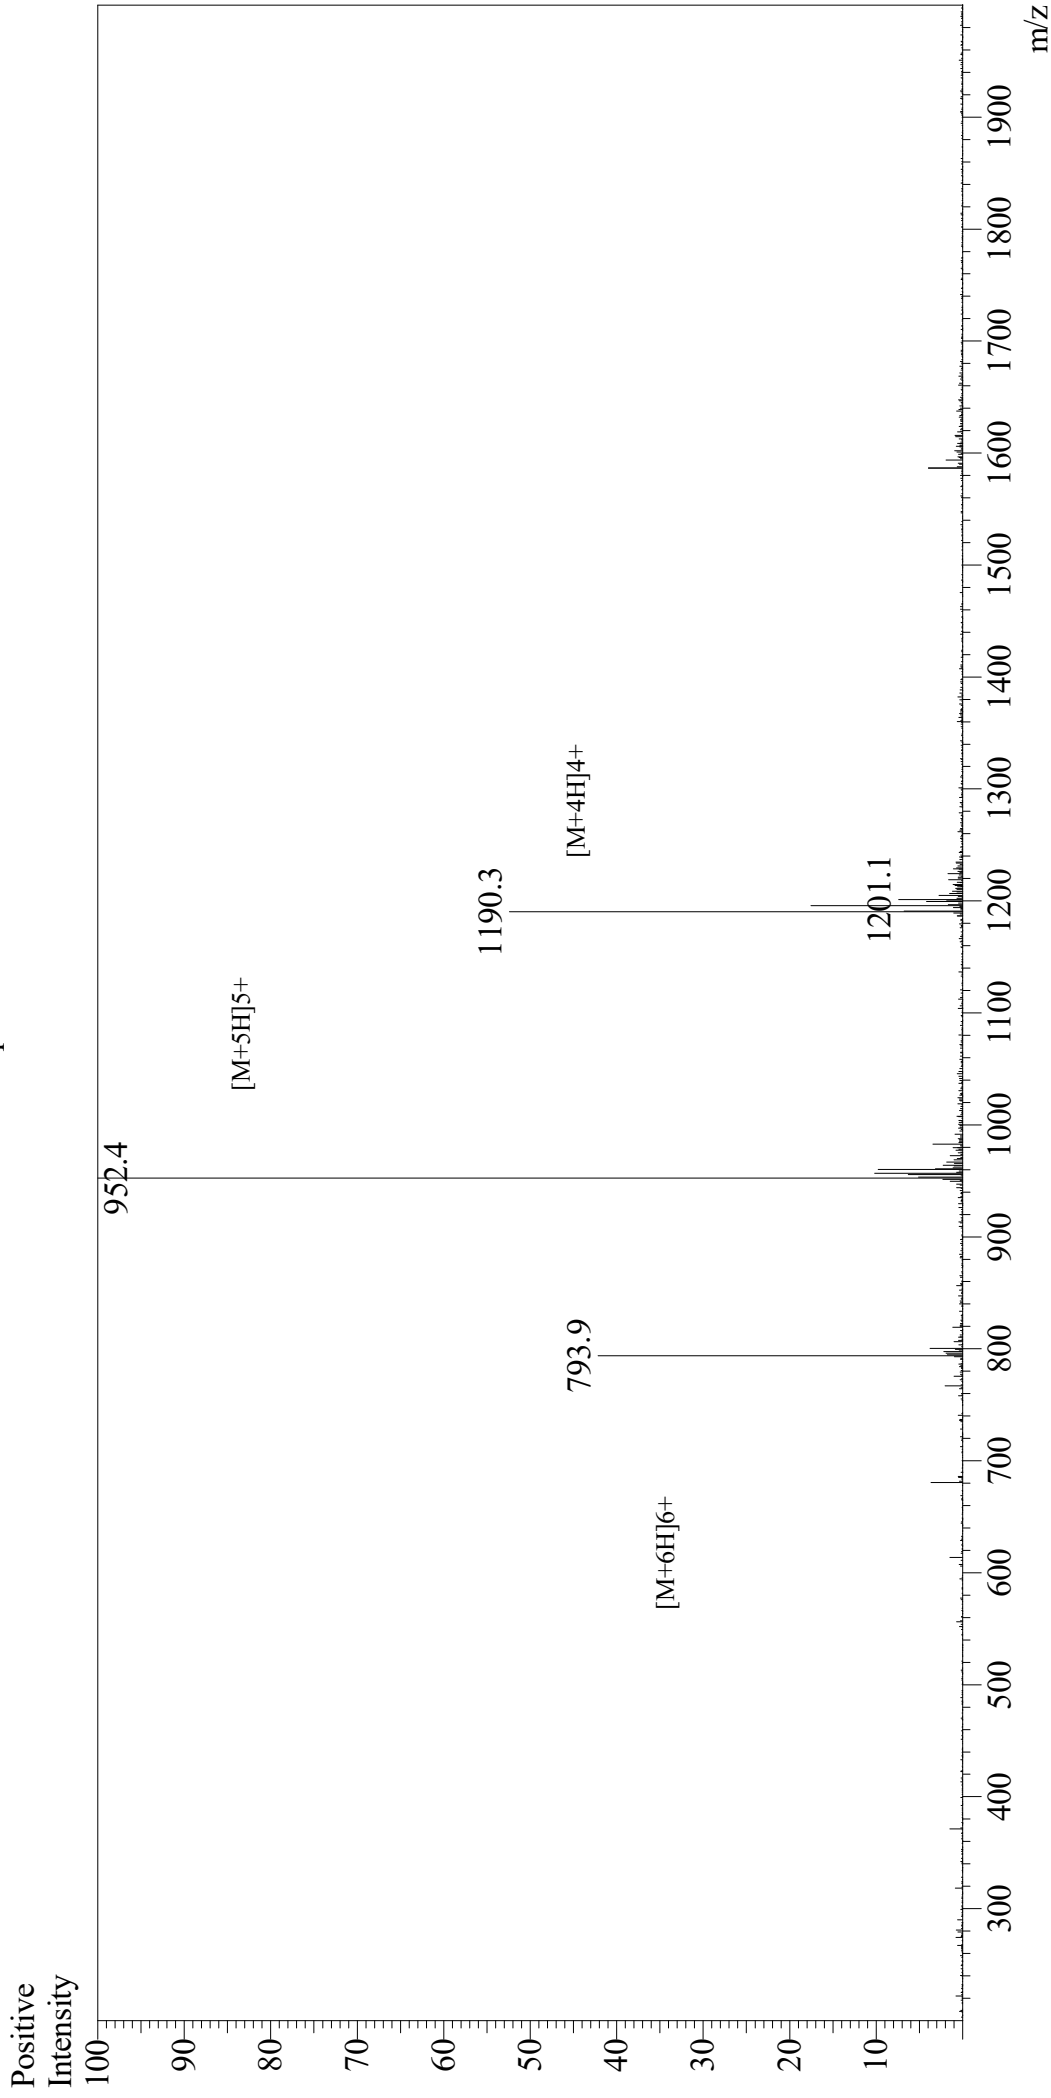

Sample Information

User : Gary
Month-Day Processed : 12/06/18
Time Processed : 10:31:04 AM
Injection Volume : 0.1
Sample Name : CRF, human, rat
Cat No. : RP10982
Lot No. : PE
Theoretical MW : 4757.45
Observed MW : 4757.0

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH