

Sample Name :Bradykinin (1-6)
 Cat No. :RP11132
 Lot No. :E0406520F
 Time Processed :14:48:12
 Month-Day-Year Processed :07/05/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

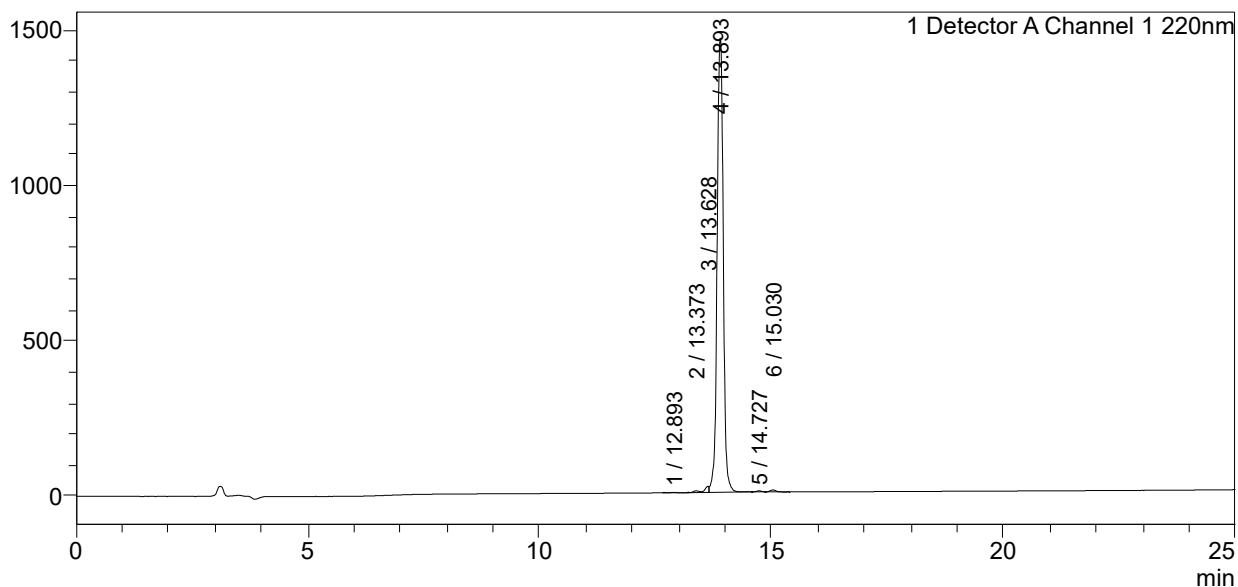

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.893	11398	1388	0.083
2	13.373	51761	5623	0.378
3	13.628	117114	19291	0.856
4	13.893	13424507	1453049	98.138
5	14.727	25004	3473	0.183
6	15.030	49417	6204	0.361
Total		13679201	1489029	100.000