

Sample Name :Arg-Gly-Asp-Ser
 Cat. No. : RP10861
 Lot. No. : PE9961807

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	0	
5.00	Pumps	Pump A B.Conc	0	
20.00	Pumps	Pump A B.Conc	30	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	0	
40.00	Pumps	Pump A B.Conc	0	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

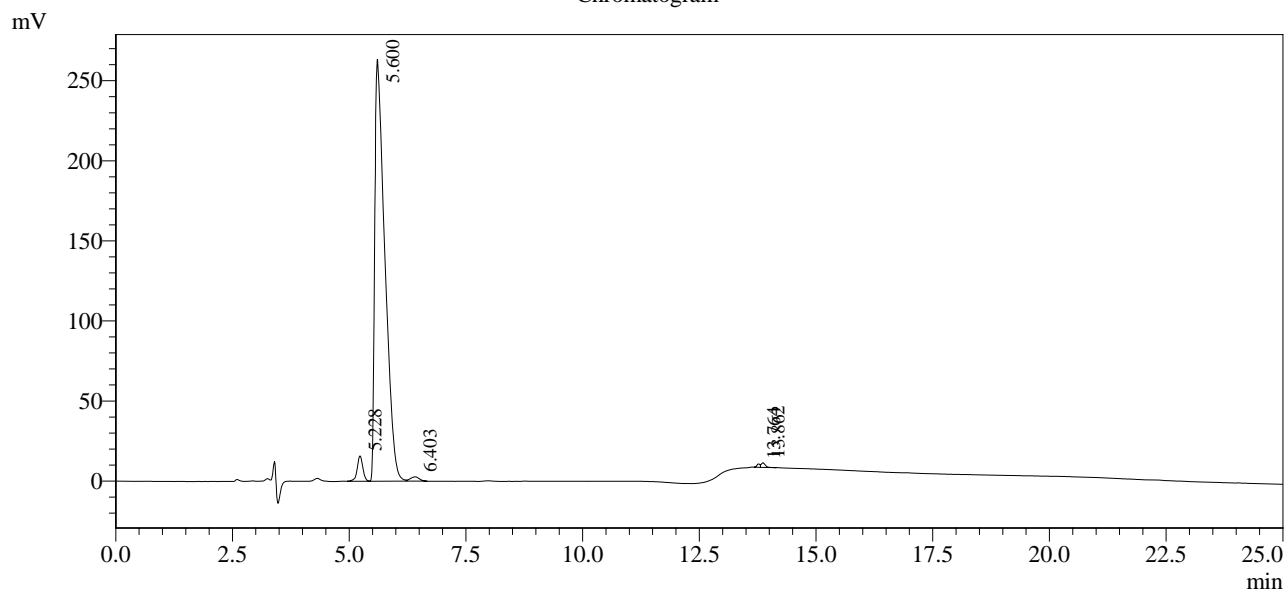

1 Det.A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.228	132770	15799	3.165
2	5.600	3998647	263362	95.318
3	6.403	35892	2735	0.856
4	13.764	10183	2124	0.243
5	13.862	17582	2909	0.419
Total		4195074	286930	100.000