

Sample Name:β-Amyloid (1-40)
 Cat No:RP10004
 Lot No :E2743820K
 Time Processed :21:32:34
 Month-Day-Year Processed :12/14/2020


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

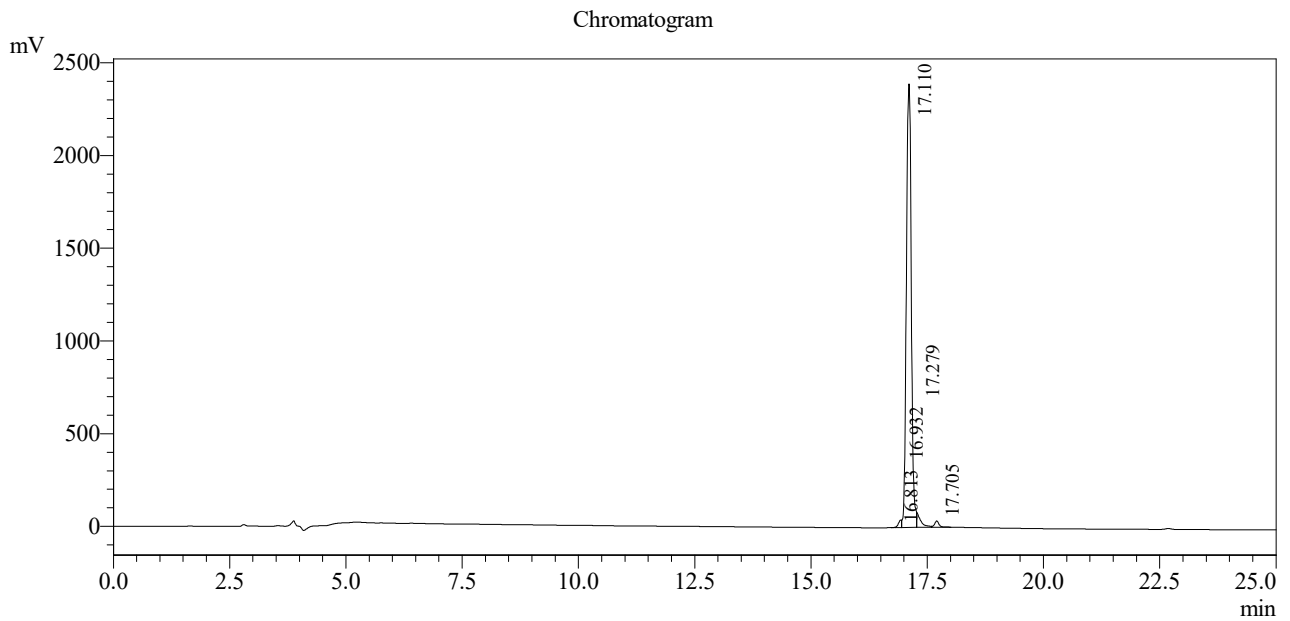

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.813	2616	1123	0.014
2	16.932	188102	40126	1.010
3	17.110	17756125	2391553	95.327
4	17.279	456701	82290	2.452
5	17.705	222958	34106	1.197
Total		18626502	2549198	100.000