

Sample Name : HA Peptide
 Cat. No. : RP11735
 Lot. No. : PE5761610

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

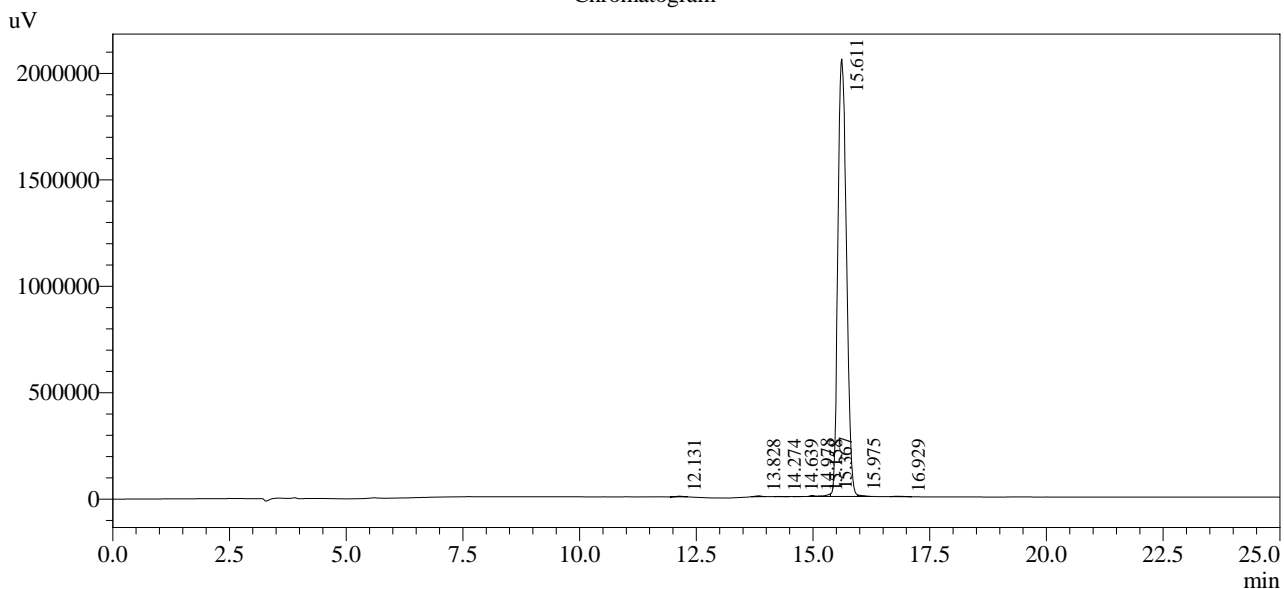

I Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.131	28652	3018	0.108
2	13.828	31509	3725	0.118
3	14.274	16894	1746	0.064
4	14.639	8069	1627	0.030
5	14.978	29287	4803	0.110
6	15.158	12227	2182	0.046
7	15.367	67697	11075	0.254
8	15.611	26345797	2055192	99.031
9	15.975	43155	5973	0.162
10	16.929	20353	1377	0.077
Total		26603639	2090717	100.000