

Sample Name :Kemptide

Cat. No. : RP10287 Lot. No. :PE2061711

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

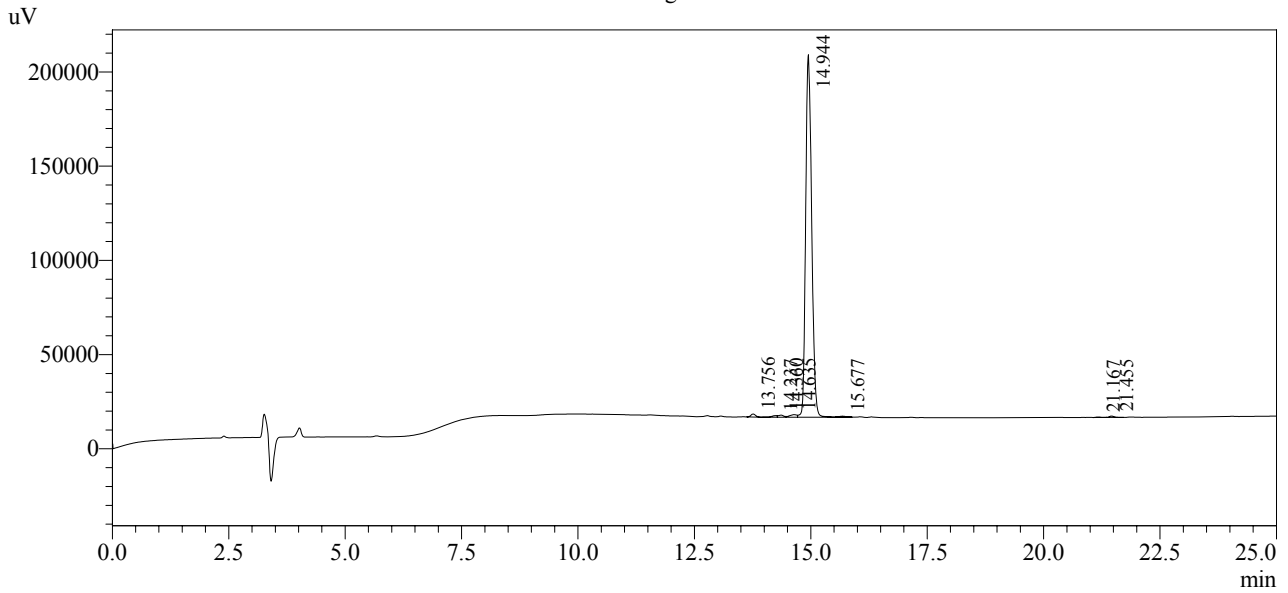

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.756	11321	1633	0.637
2	14.237	6587	810	0.371
3	14.360	8486	1095	0.477
4	14.635	14108	1320	0.794
5	14.944	1724959	192314	97.035
6	15.677	5048	520	0.284
7	21.167	1786	259	0.100
8	21.455	5376	754	0.302
Total		1777670	198706	100.000