

Sample Name :  $\beta$ -amyloid (12-28)  
 Cat No.: RP20104  
 Lot No.: E9612619L  
 Time Processed :21:39:39  
 Month-Day-Year Processed :12/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
95.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

<Chromatogram>

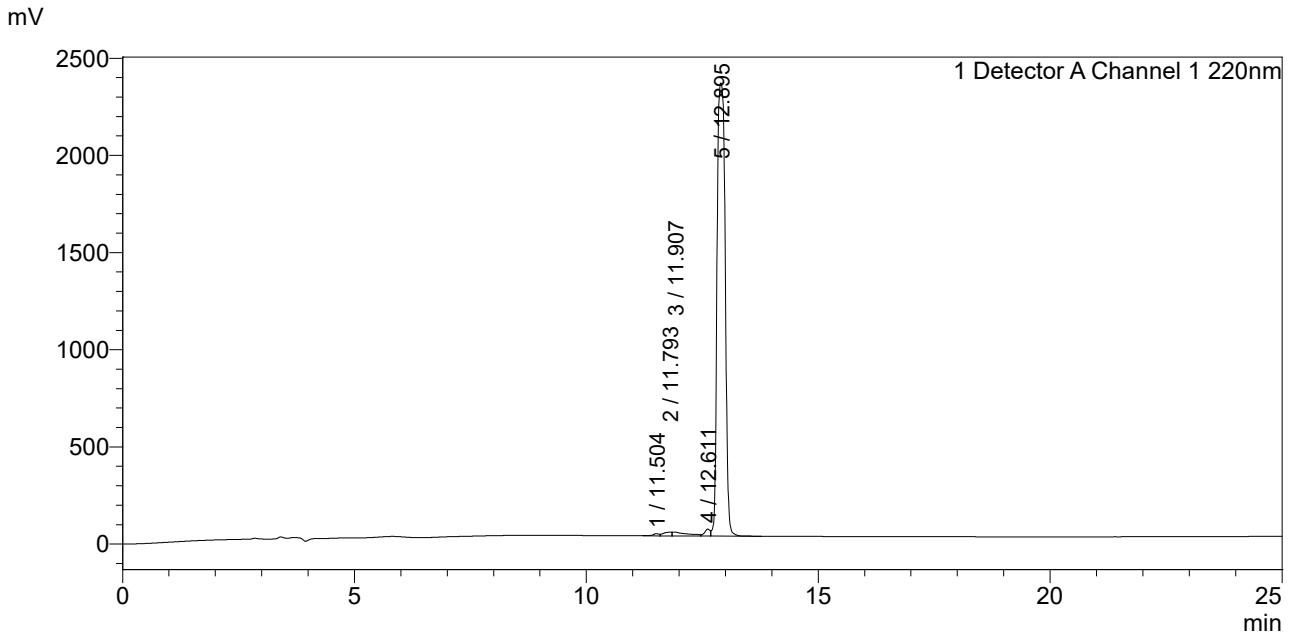

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.504	105859	11349	0.364
2	11.793	242460	18946	0.833
3	11.907	449659	19590	1.545
4	12.611	296109	36005	1.017
5	12.895	28017449	2332256	96.242
Total		29111536	2418147	100.000