

Sample Name:CLIP (86-100)
 Cat. No. : RP20279
 Lot. No. : E1561820A
 Time Processed: 9:01:37 AM
 Month-Day-Year Processed :01/19/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Equipment:ZJ19010325

<Chromatogram>

mV

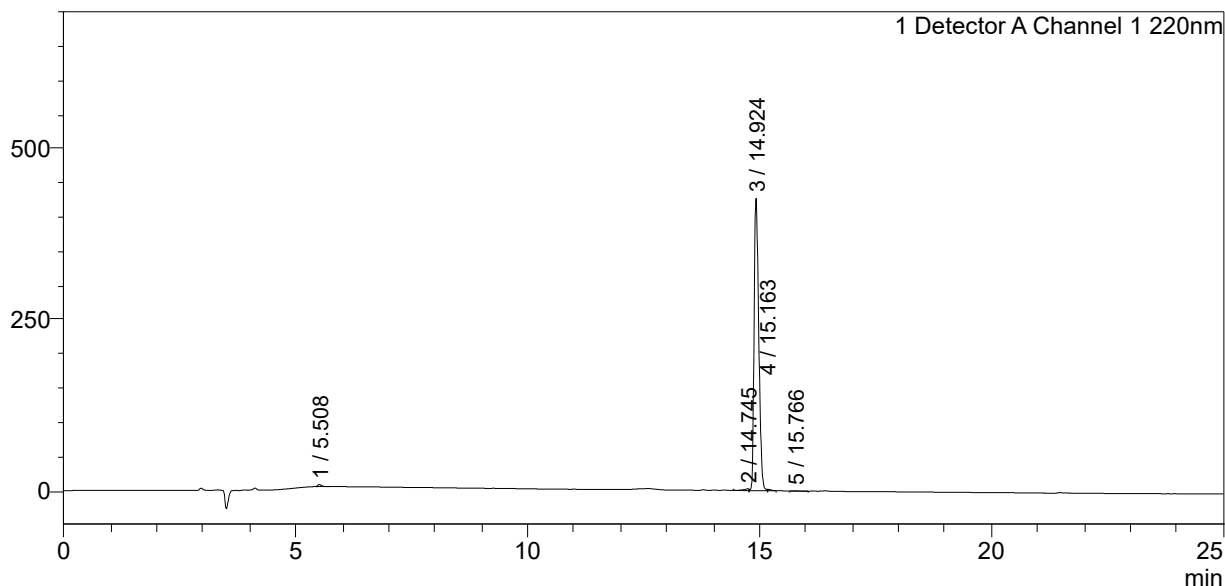

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.508	14503	2744	0.475
2	14.745	22242	2566	0.728
3	14.924	3002905	427521	98.288
4	15.163	11376	1898	0.372
5	15.766	4184	313	0.137
Total		3055210	435042	100.000