


# Mass Spectrum

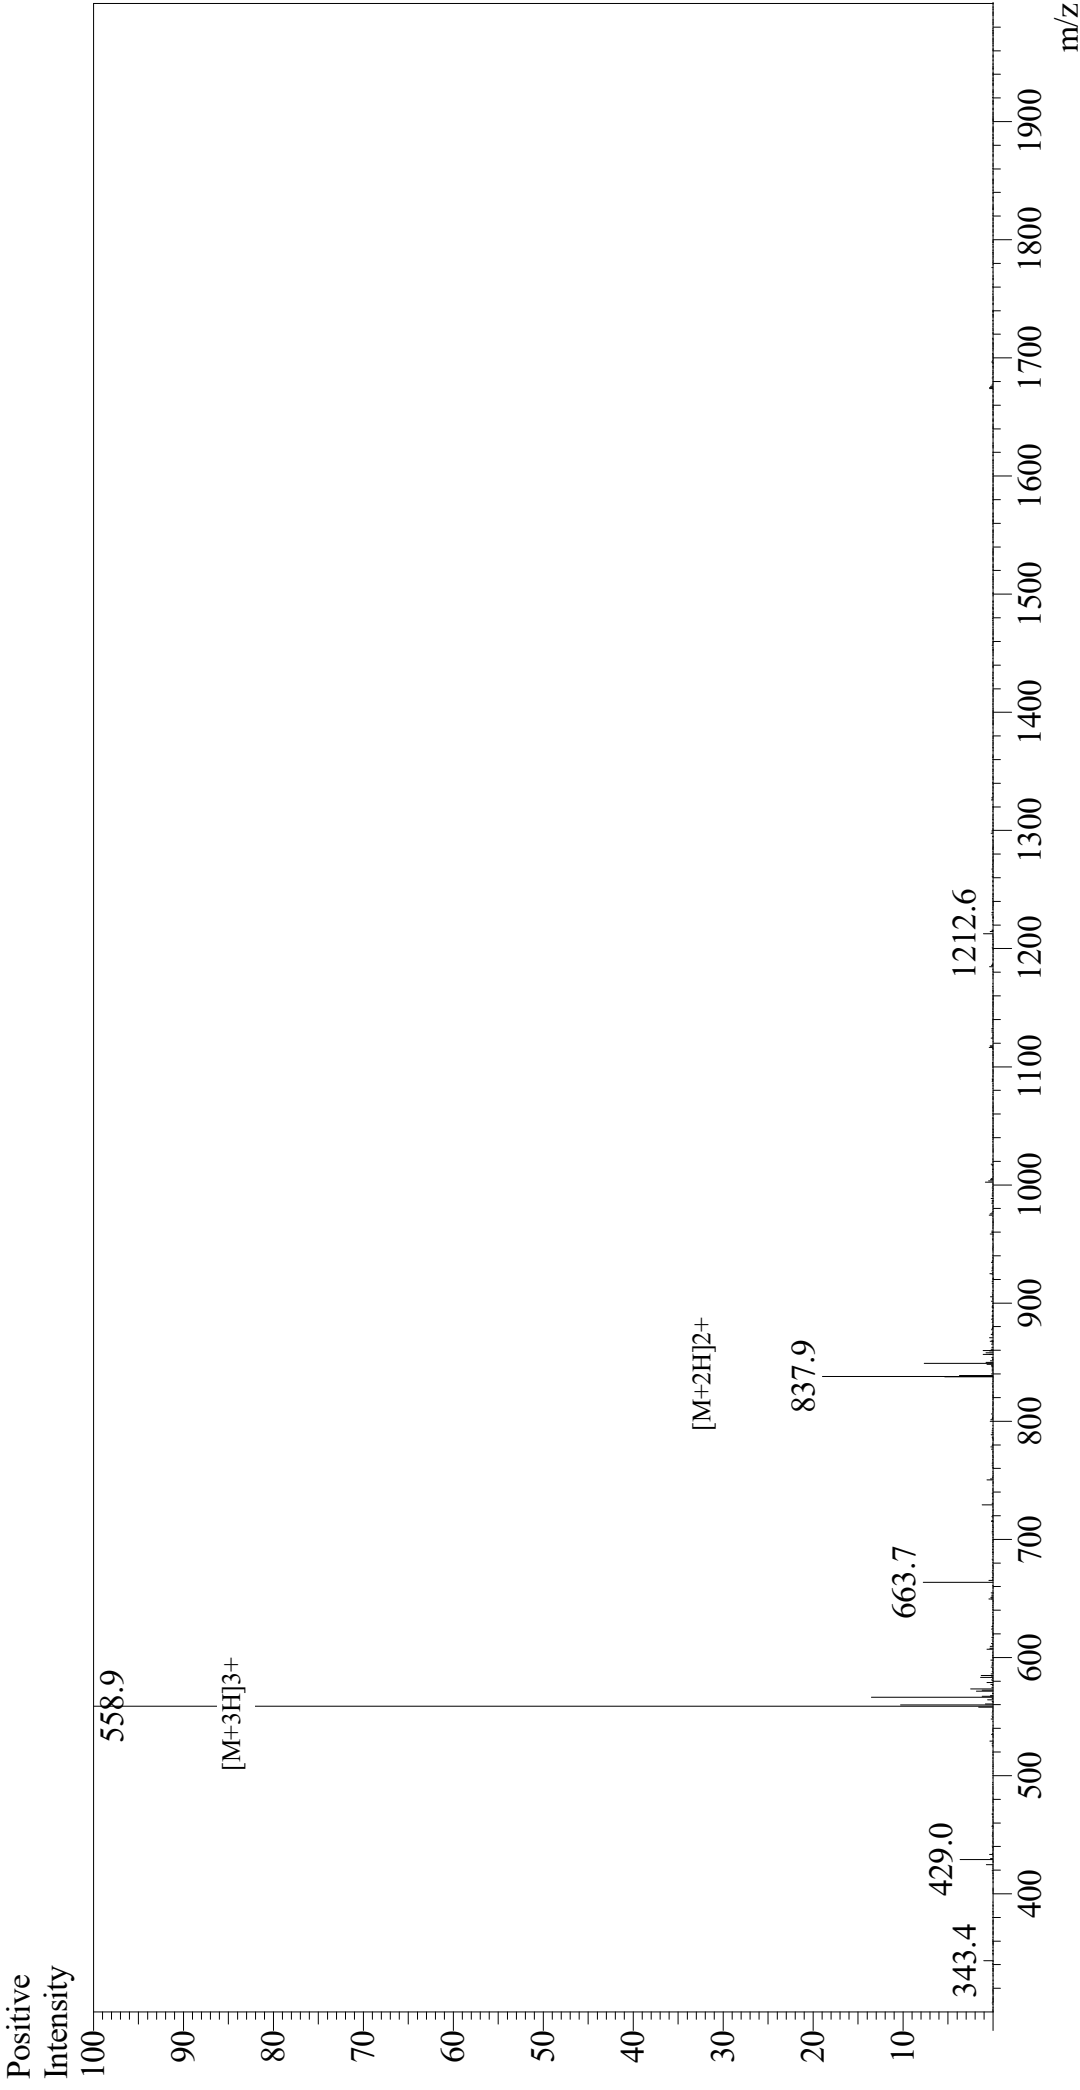

## Sample Information

Acquired by : Gary  
Month-Day Processed : 01/18/20  
Time Processed : 09:25:51 PM  
Injection Volume : 0.3  
Sample Name : CLIP (86-100)  
Cat. No. : RP20279  
Lot. No. : E1561820A  
Theoretical MW : 1674.10  
Observed MW : 1673.7

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200

Equipment : GK11010007  
Interface Bias : +4.5 kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2 ml/min  
B.conc : 50%H2O/50%MeOH