

Sample Name :β-amyloid (1-11)
 Cat No. :RP20105
 Lot No. :E4830319I
 Time Processed :6:25:27 PM
 Month-Day-Year Processed :09/21/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

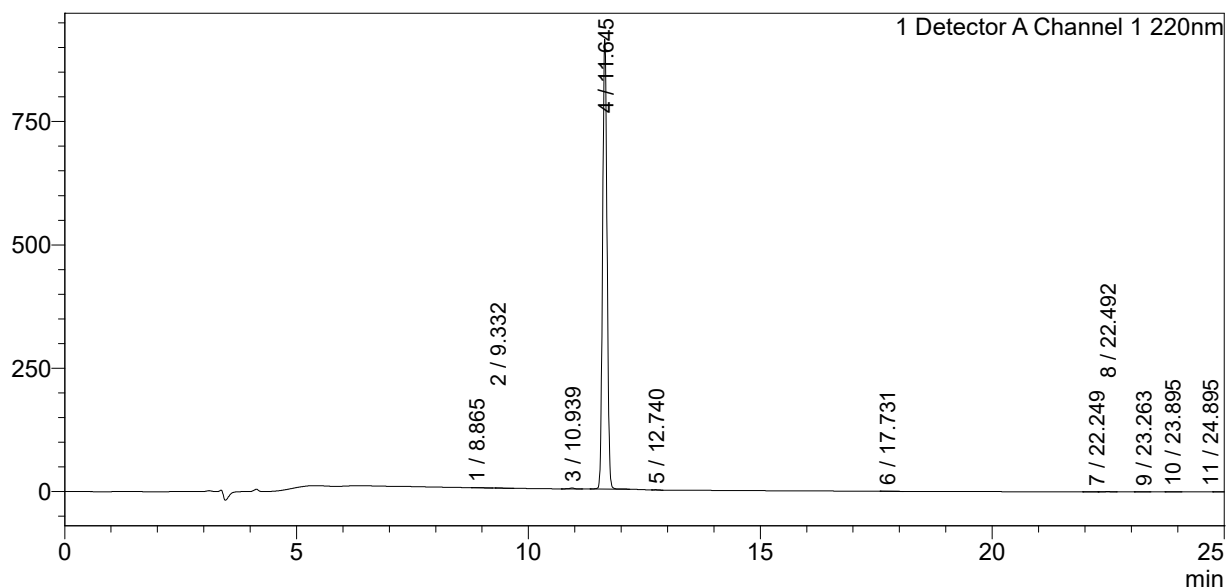

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.865	4036	264	0.066
2	9.332	1185	83	0.019
3	10.939	18017	2312	0.293
4	11.645	6097705	912102	99.292
5	12.740	3597	630	0.059
6	17.731	3573	315	0.058
7	22.249	1959	151	0.032
8	22.492	7153	604	0.116
9	23.263	1185	104	0.019
10	23.895	1191	87	0.019
11	24.895	1595	199	0.026
Total		6141197	916851	100.000