

Sample Name :N-Acetyl-Ser-Asp-Lys-Pro
 Cat No.: RP10555
 Lot No.: E4745219I
 Time Processed :9:54:16
 Month-Day-Year Processed :09/22/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
5.00	Pumps	Solvent B Conc.	0
20.00	Pumps	Solvent B Conc.	30
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	0
33.00	Pumps	Solvent B Conc.	0
33.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

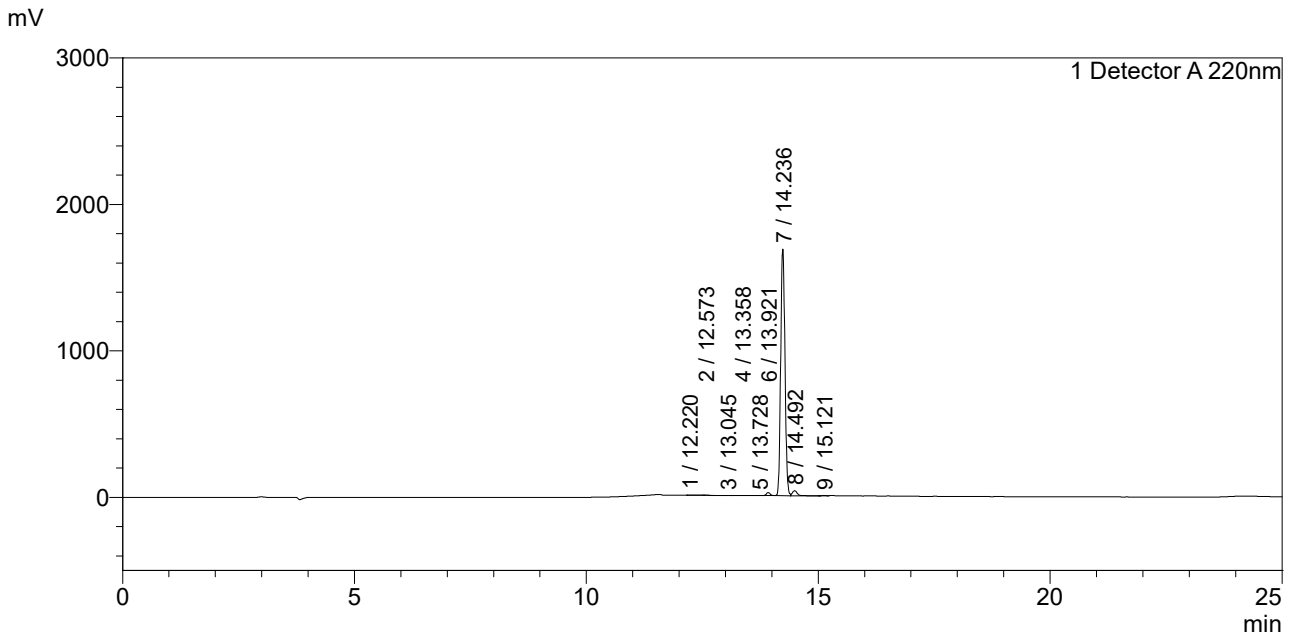

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.220	1964	111	0.017
2	12.573	2915	228	0.026
3	13.045	2839	572	0.025
4	13.358	21037	1172	0.187
5	13.728	8094	1064	0.072
6	13.921	125031	21212	1.112
7	14.236	10828237	1685266	96.332
8	14.492	241056	35013	2.145
9	15.121	9332	1502	0.083
Total		11240504	1746141	100.000