

Sample Name :Proctolin
 Cat. No. :RP10475
 Lot. No. : PE0511706


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

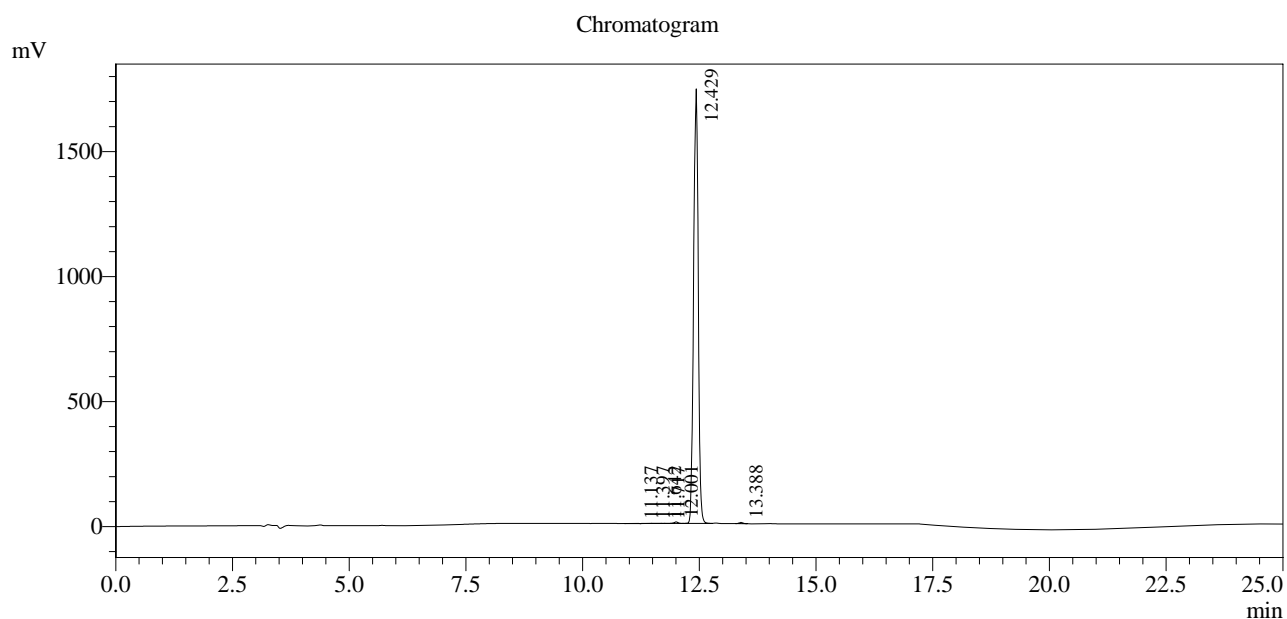

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.137	1120	129	0.009
2	11.397	676	99	0.006
3	11.642	1260	166	0.010
4	11.717	831	196	0.007
5	12.001	39368	6069	0.323
6	12.429	12100450	1738273	99.425
7	13.388	26692	4732	0.219
Total		12170398	1749663	100.000