

Sample Name : β -Amyloid (31-35)
 Cat No. :RP20184
 Lot No. :E4830119I
 Time Processed :15:03:02
 Month-Day-Year Processed :09/30/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

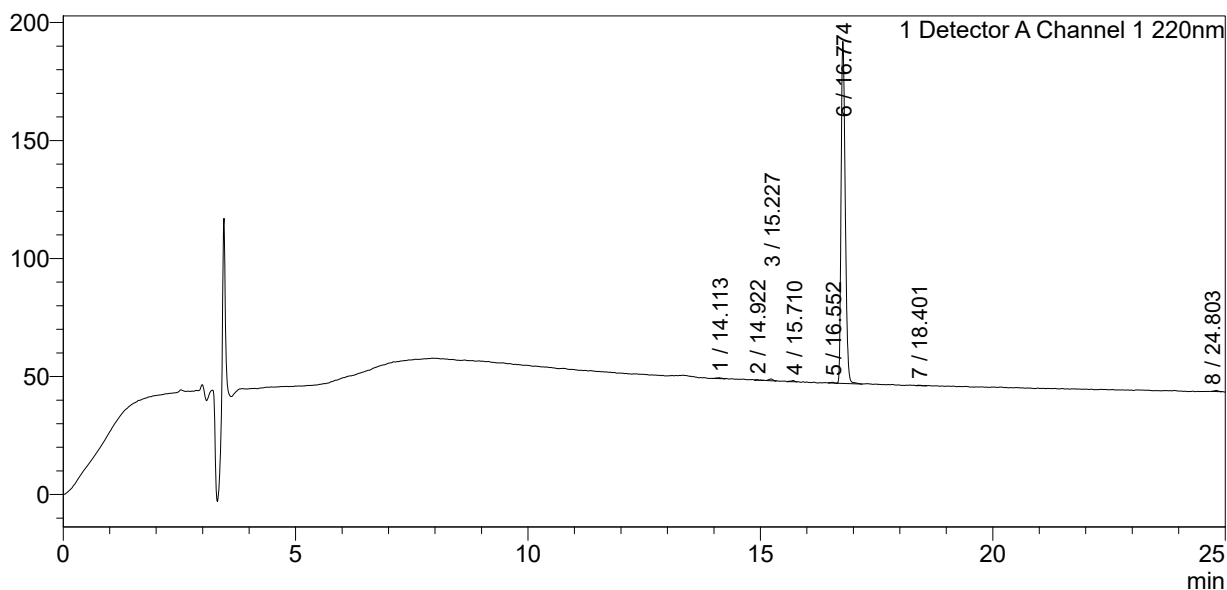

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.113	2886	433	0.314
2	14.922	1138	267	0.124
3	15.227	4459	768	0.485
4	15.710	2743	480	0.298
5	16.552	1795	359	0.195
6	16.774	902651	144858	98.162
7	18.401	1136	227	0.124
8	24.803	2747	463	0.299
Total		919556	147855	100.000