

Sample Name:RGD
 Cat No.: RP20297
 Lot No.:E6825820H
 Time Processed :14:15:34
 Month-Day-Year Processed :08/08/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	55
25.10	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
50.00	Pumps	Pump A B.Conc	15
51.00	Pumps	Pump A B.Conc	15
95.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

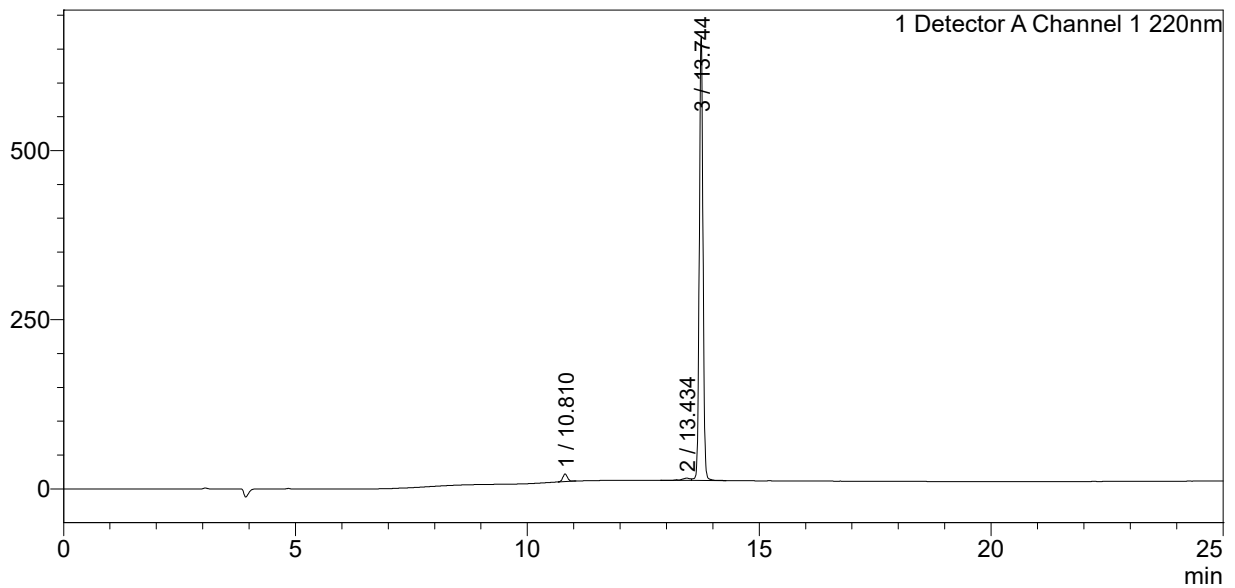

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.810	78520	11139	2.074
2	13.434	43909	3448	1.160
3	13.744	3662715	657034	96.766
Total		3785144	671621	100.000