

Sample Name :Syntide 2
 Cat No. :RP10322
 Lot No. :E5742220B
 Time Processed :9:13:08
 Month-Day-Year Processed :02/08/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
32.00	Pumps	Solvent B Conc.	95
32.01	Pumps	Solvent B Conc.	5
41.00	Pumps	Solvent B Conc.	5
41.00	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

mV

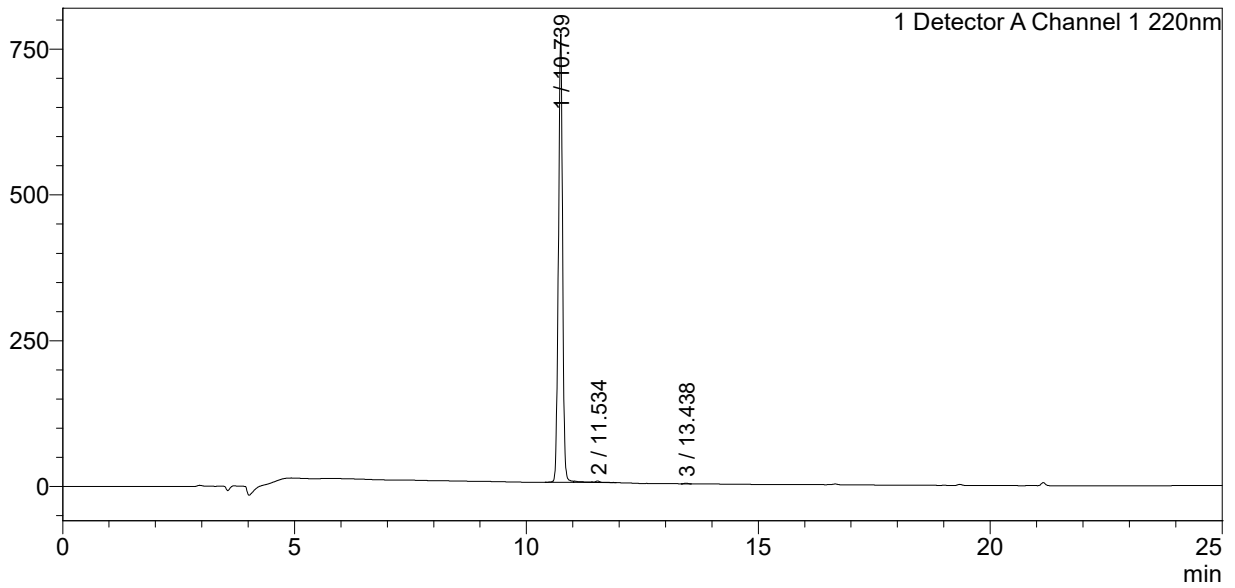

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.739	4792195	769146	98.894
2	11.534	47648	2463	0.983
3	13.438	5929	1134	0.122
Total		4845772	772744	100.000