

Sample Name : Cardiotoxin Analog (CTX) IV (6-12)
 Cat.No : RP17303
 Lot.No : E3653920J
 Time Processed: 5:42:43
 Year-Month-Day: 2020/11/3

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>


Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
33.00	Pumps	Solvent B Conc.	5	
33.01	Controller	Stop		

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010015

<Chromatogram>

mV

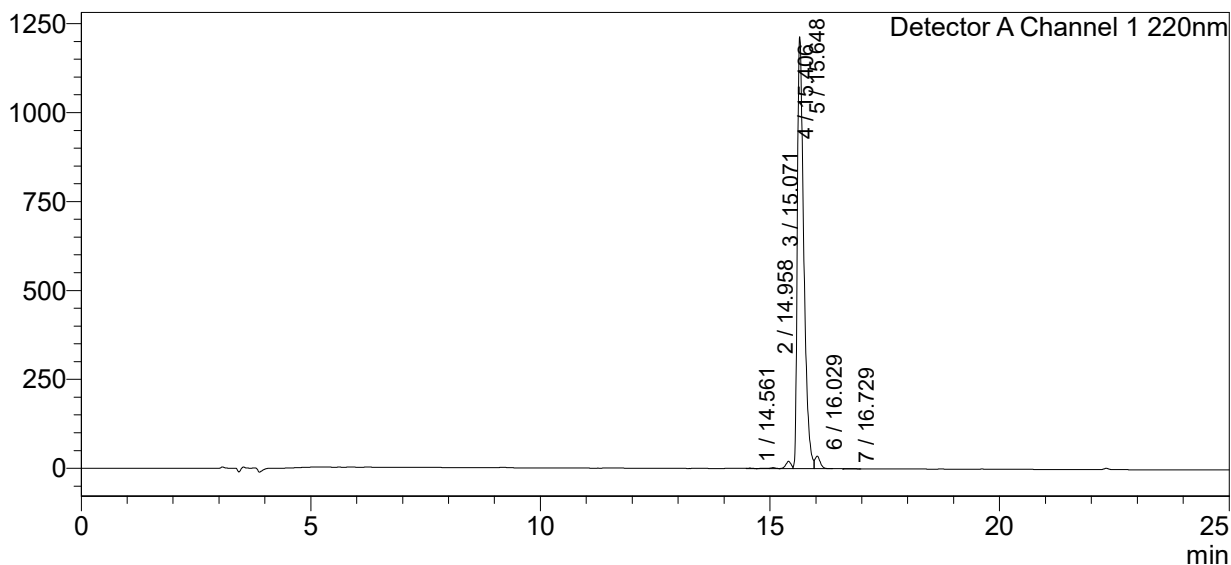

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.561	8692	1214	0.071
2	14.958	8990	957	0.073
3	15.071	16777	2477	0.136
4	15.406	164109	20612	1.334
5	15.648	11818245	1214031	96.045
6	16.029	280845	35064	2.282
7	16.729	7233	720	0.059
Total		12304891	1275074	100.000