

Sample Name :LL37 (Human)  
 Cat No. :RP13323  
 Lot No. :E2885120L  
 Time Processed :7:41:22  
 Month-Day-Year Processed :12/23/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

### <Chromatogram>

mV

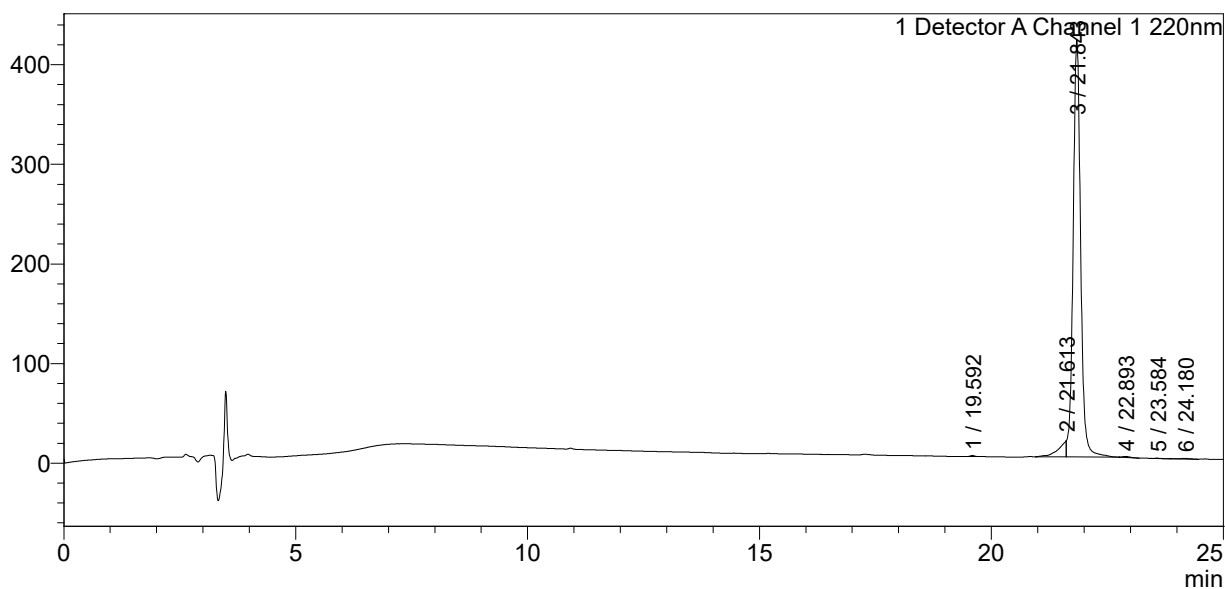

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	19.592	7507	1061	0.152
2	21.613	196851	15834	3.985
3	21.843	4710503	419099	95.365
4	22.893	11459	1135	0.232
5	23.584	2867	290	0.058
6	24.180	10250	725	0.208
Total		4939438	438144	100.000