

Sample Name :Fibronectin CS1 Peptide  
 Cat No.:RP10838  
 Lot No.: E4778919I  
 Time Processed :8:53:21  
 Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

### <Chromatogram>

mV

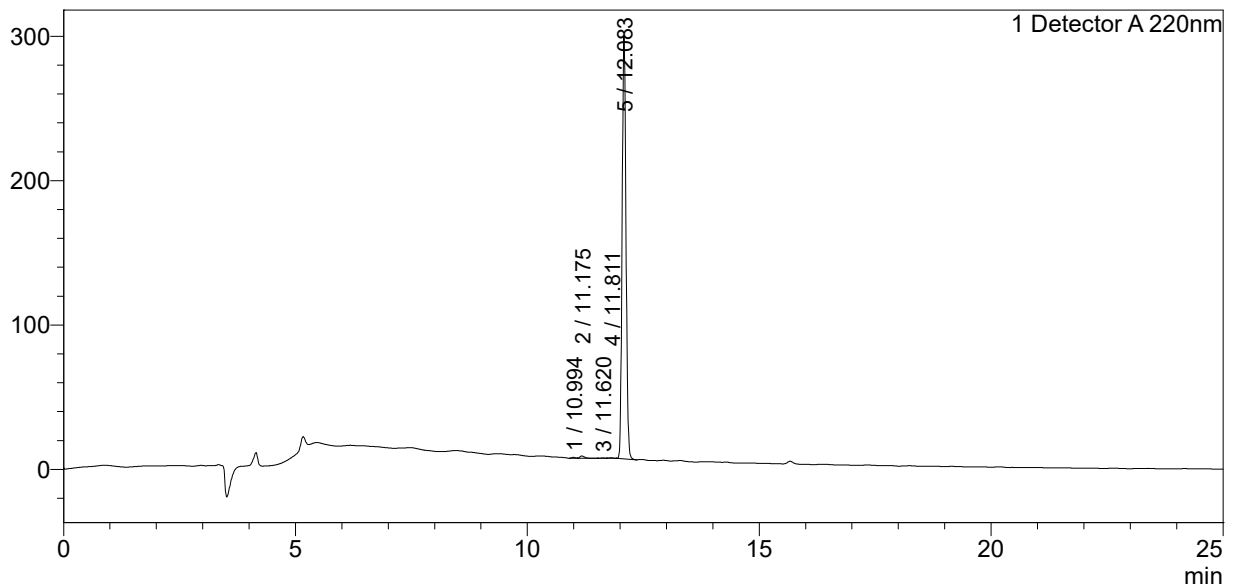

### <Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.994	3747	654	0.218
2	11.175	11391	1612	0.663
3	11.620	1482	221	0.086
4	11.811	2837	400	0.165
5	12.083	1698654	293000	98.868
Total		1718111	295888	100.000