

Sample Name :Hexa-His
 Cat No. :RP11737
 Lot No. :E6457219G
 Time Processed :6:21:30 PM
 Month-Day-Year Processed :07/25/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
5.00	Pumps	Solvent B Conc.	0
20.00	Pumps	Solvent B Conc.	30
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	0
35.00	Pumps	Solvent B Conc.	0
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ19010141

<Chromatogram>

mV

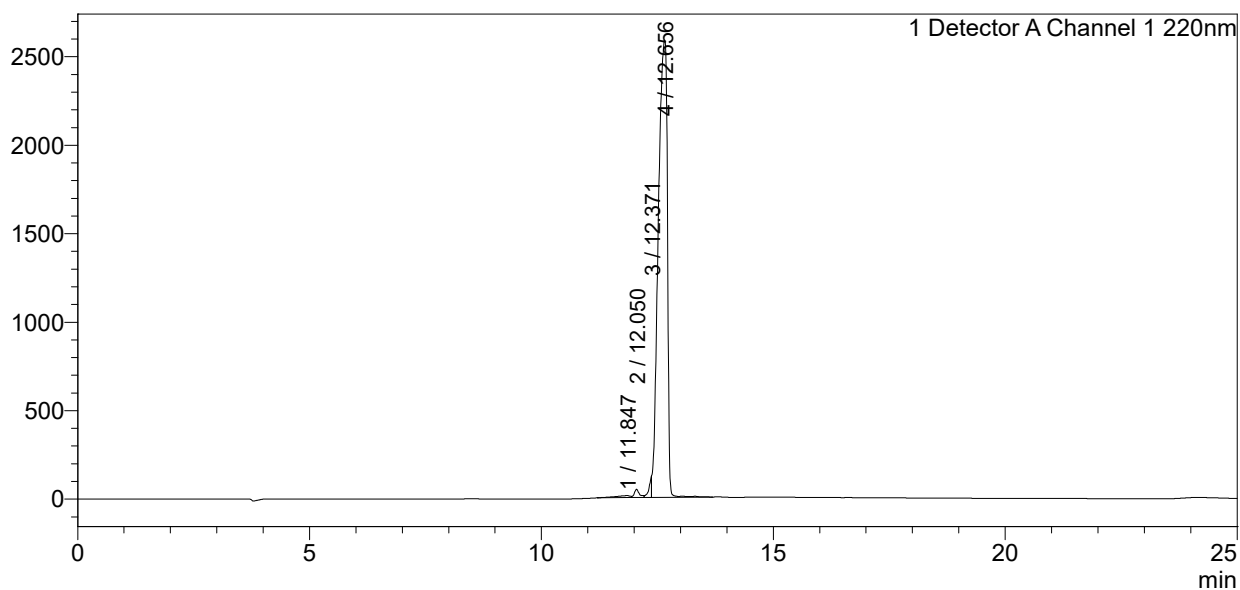

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.847	262573	11370	0.728
2	12.050	356197	46744	0.987
3	12.371	464523	113522	1.288
4	12.656	34991769	2585549	96.997
Total		36075062	2757186	100.000