

Sample Name :PTD-p65-P1 Peptide
Cat No. :RP20522
Lot No. :E7107919J
Time Processed :2:28:45 AM
Month-Day-Year Processed :10/03/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
Equipment: ZJ19010141

<Chromatogram>

mV

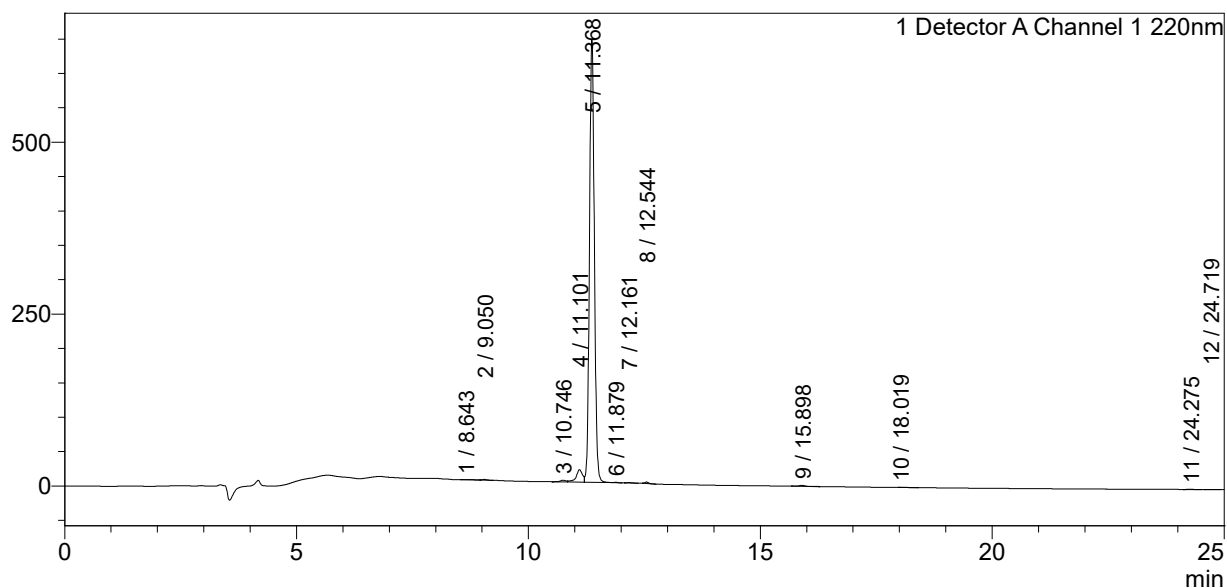

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.643	2481	192	0.051
2	9.050	5240	900	0.107
3	10.746	22649	2481	0.462
4	11.101	174880	18167	3.565
5	11.368	4666352	644668	95.117
6	11.879	3048	607	0.062
7	12.161	3735	490	0.076
8	12.544	10541	2029	0.215
9	15.898	12358	1436	0.252
10	18.019	1608	65	0.033
11	24.275	1787	128	0.036
12	24.719	1243	113	0.025
Total		4905923	671275	100.000