


Mass Spectrum

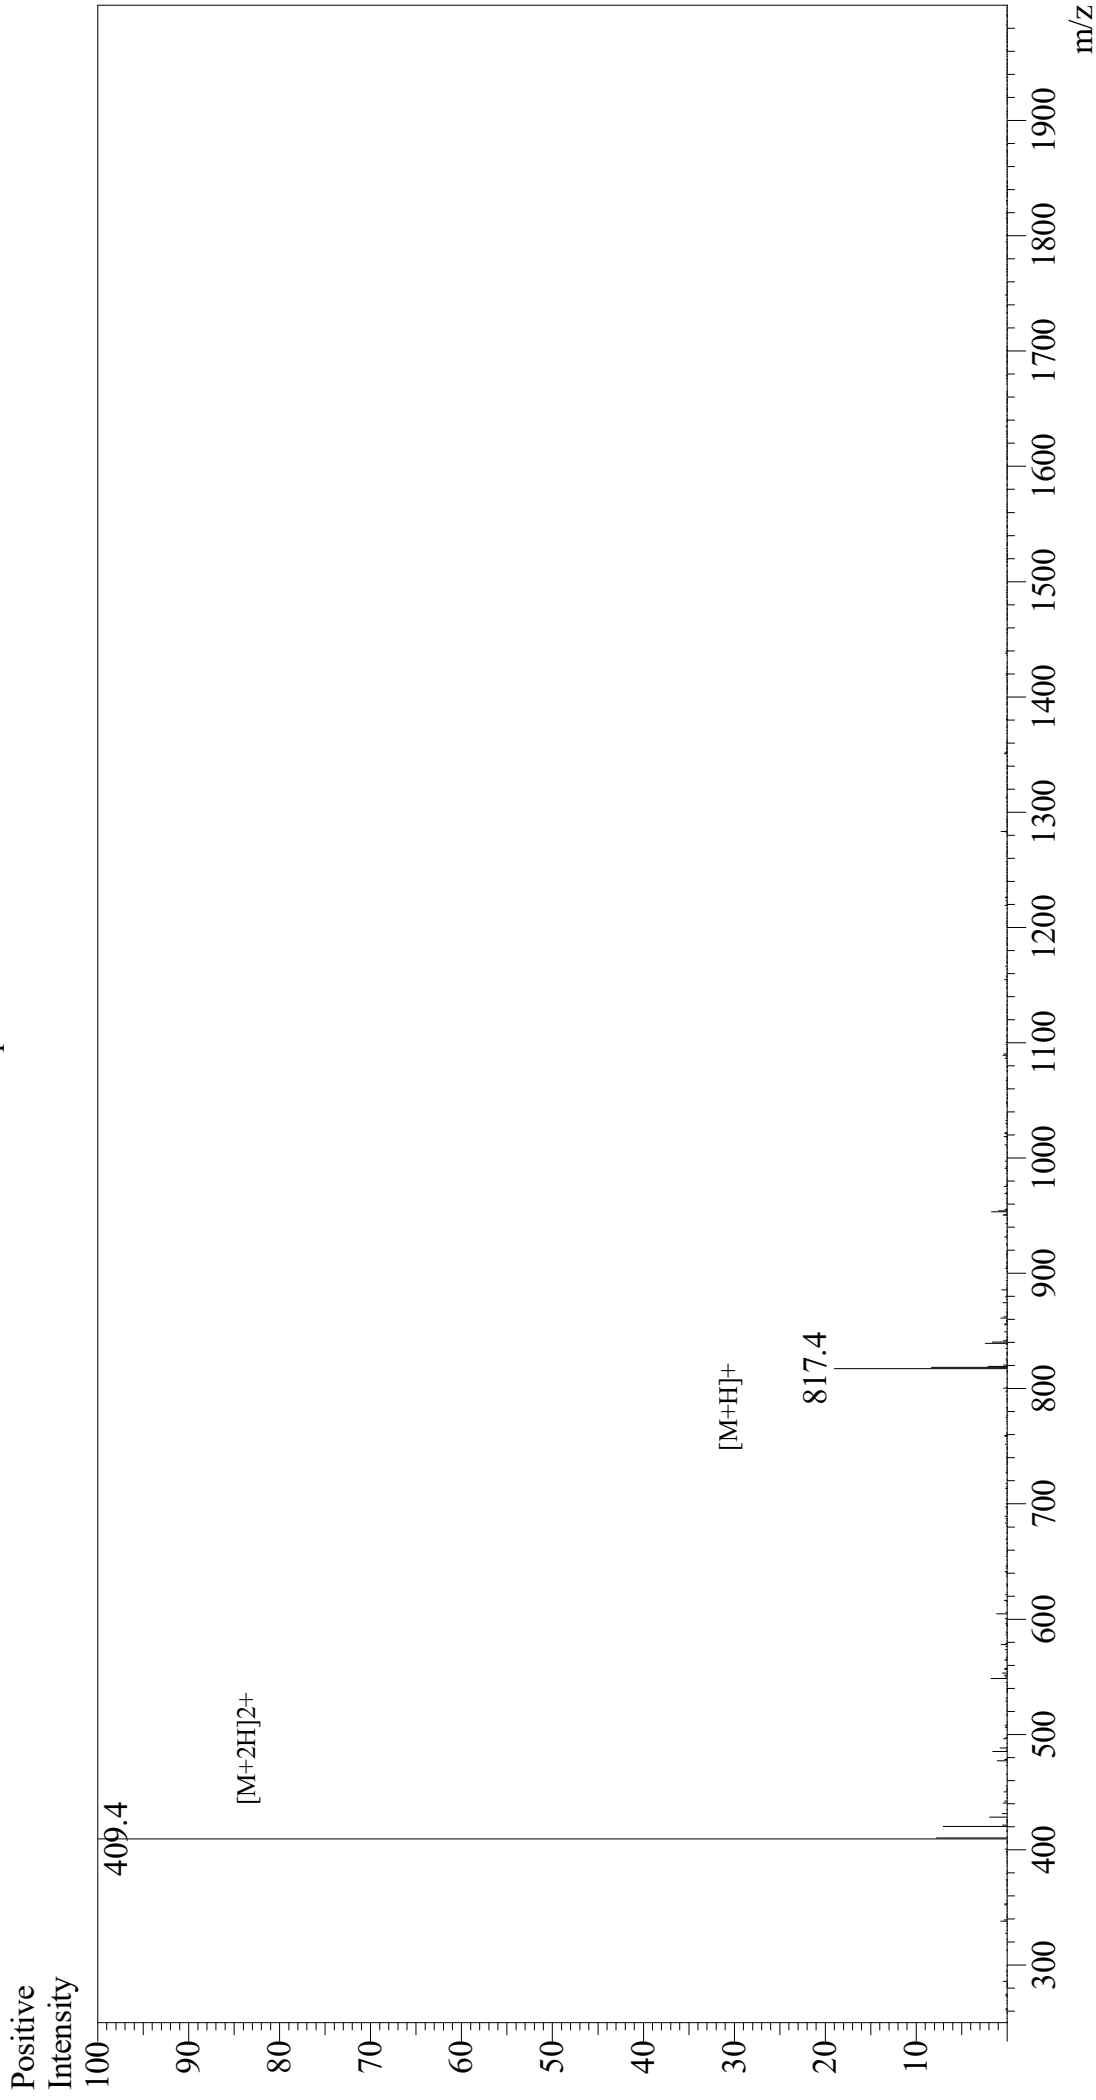

Sample Information

Month-Day Processed : 12/01/20
Time Processed : 03:27:17 PM
Injection Volume : 0.3
Sample Name : Neutensin (8-13)
Cat No. : RP10442
Lot No. : E2688620K
Theoretical MW : 816.99
Observed MW : 816.8

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH