

Sample Name :Axl tide
 Cat. No. :RP20363
 Lot. No. : PE19011810
 Time Processed : 8:37:24
 Month-Day-Year Processed : 10/11/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

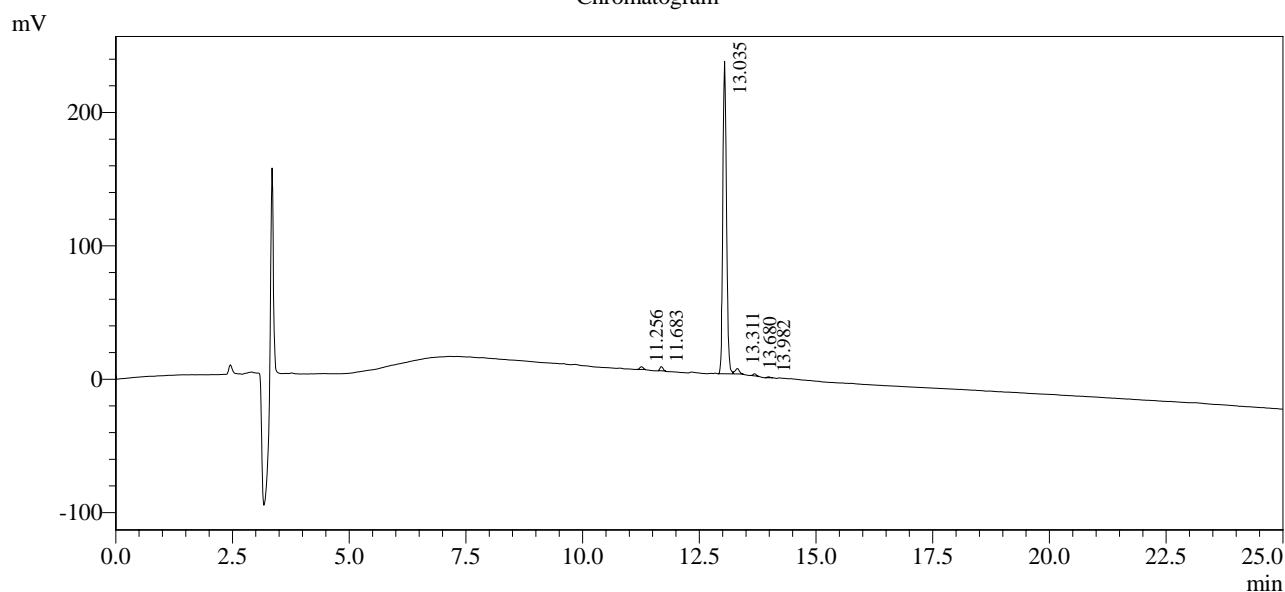

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.256	10141	2027	0.751
2	11.683	14584	3128	1.079
3	13.035	1290556	234358	95.516
4	13.311	25789	4089	1.909
5	13.680	7198	1525	0.533
6	13.982	2878	679	0.213
Total		1351146	245806	100.000