

Sample Name : HPV16 E7(86-93)  
 Cat No. : RP20499  
 Lot No. : E5697519F  
 Time Processed : 17:00:28  
 Month-Day-Year Processed : 06/29/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: GK12010012

### <Chromatogram>

mV

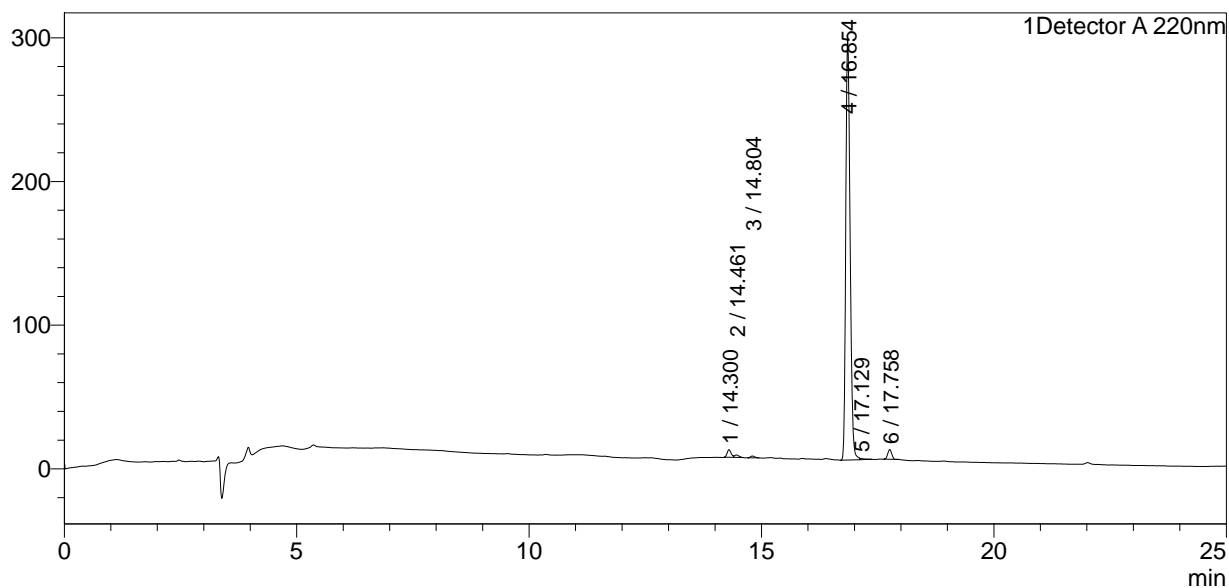

### <Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.300	31634	5310	1.576
2	14.461	11030	1689	0.549
3	14.804	7943	1279	0.396
4	16.854	1911945	293343	95.224
5	17.129	5168	867	0.257
6	17.758	40110	6816	1.998
Total		2007830	309302	100.000