

Sample Name : β -Amyloid (1-40)
 Cat. No. : RP10004
 Lot. No. : E8640220L
 Time Processed :3:27:42 PM
 Month-Day-Year Processed :12/07/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

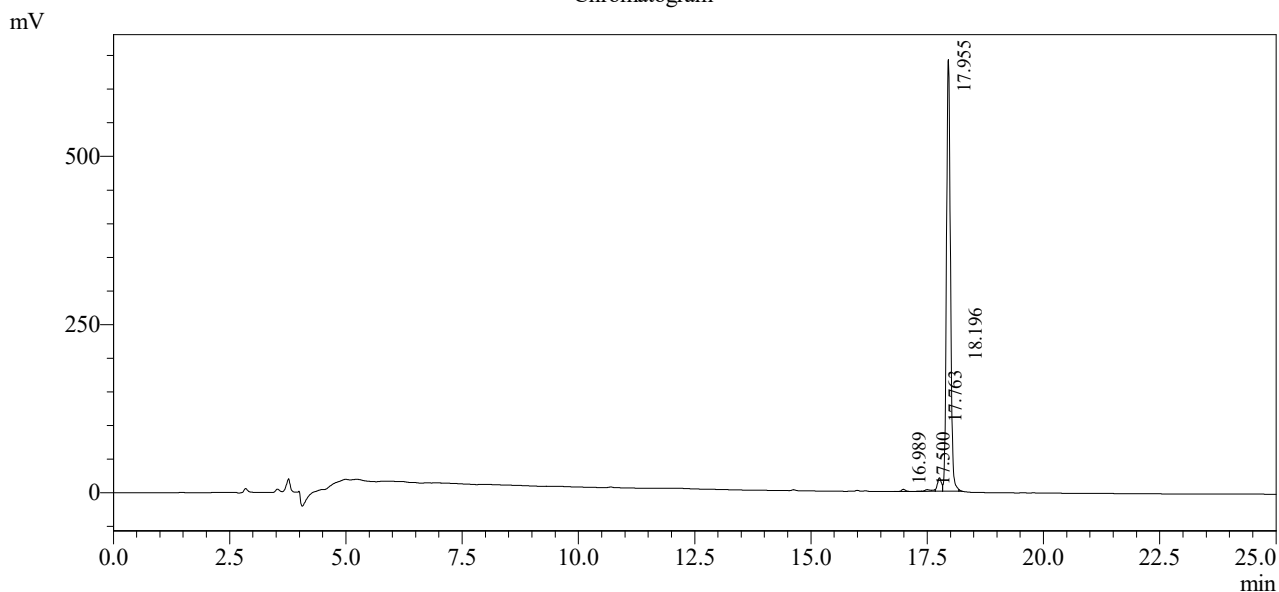

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.989	22119	3263	0.555
2	17.500	28709	2439	0.720
3	17.763	120677	19841	3.027
4	17.955	3813083	641468	95.648
5	18.196	1973	1500	0.049
Total		3986561	668511	100.000