

Sample Name :Hexa-His  
 Cat. No. : RP11737  
 Lot. No. : E7095921A  
 Time Processed :4:43:19 PM  
 Month-Day-Year Processed :01/16/2021  
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	0
5.00	Pumps	Pump A B.Conc	0
20.00	Pumps	Pump A B.Conc	30
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	0
35.00	Pumps	Pump A B.Conc	0
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: GR11010440

<Chromatogram>

mV

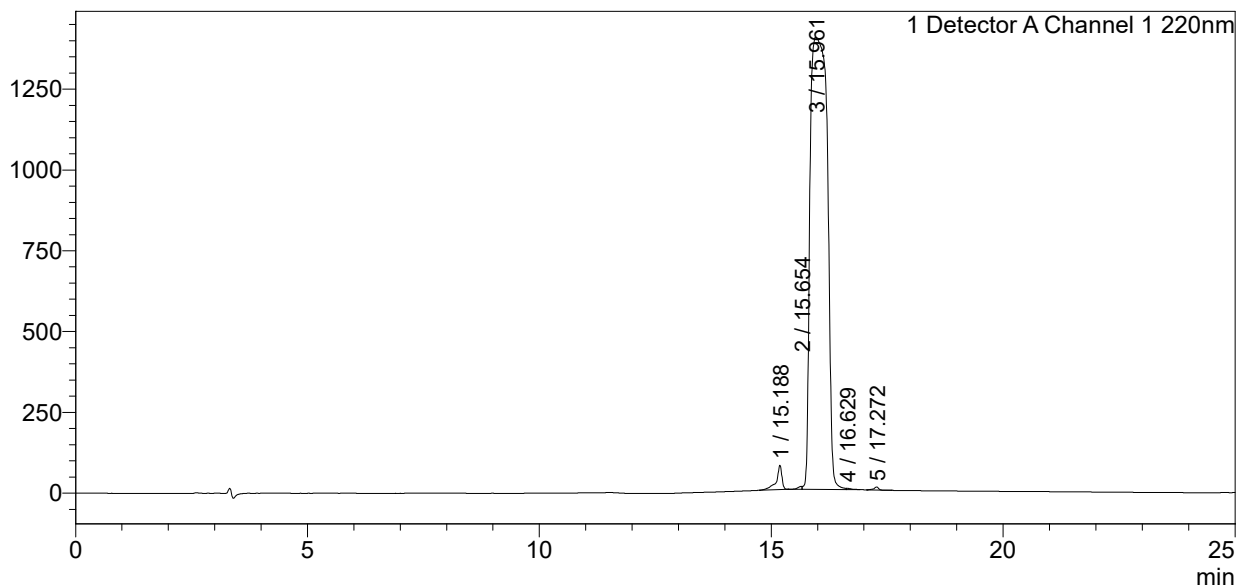

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.188	622975	75187	1.707
2	15.654	58437	9084	0.160
3	15.961	35725788	1399296	97.883
4	16.629	26041	3473	0.071
5	17.272	65249	9619	0.179
Total		36498489	1496659	100.000