

Sample Name :Atrial Natriuretic Peptide (ANP) (1-28), human, porcine

Cat. No. : RP11927

Lot. No. : E3608321B

Time Processed :8:14:05 AM

Month-Day-Year Processed :02/09/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ17010508

<Chromatogram>

mV

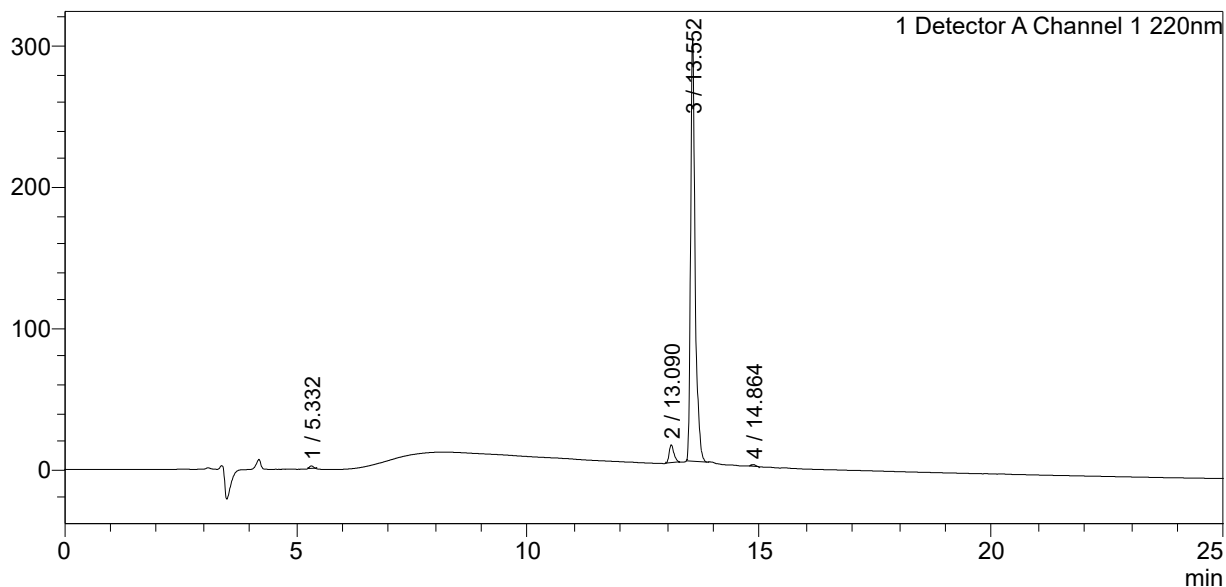

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.332	9841	1824	0.460
2	13.090	89255	12680	4.174
3	13.552	2032787	299903	95.067
4	14.864	6389	1125	0.299
Total		2138273	315532	100.000