

Sample Name : Arg-Gly-Asp-Ser
 Cat No.: RP10861
 Lot No.: E0635521A
 Time Processed : 7:12:41
 Month-Day-Year Processed : 01/31/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
5.00	Pumps	Solvent B Conc.	0
20.00	Pumps	Solvent B Conc.	30
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	0
40.00	Pumps	Solvent B Conc.	0
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010014

<Chromatogram>

mV

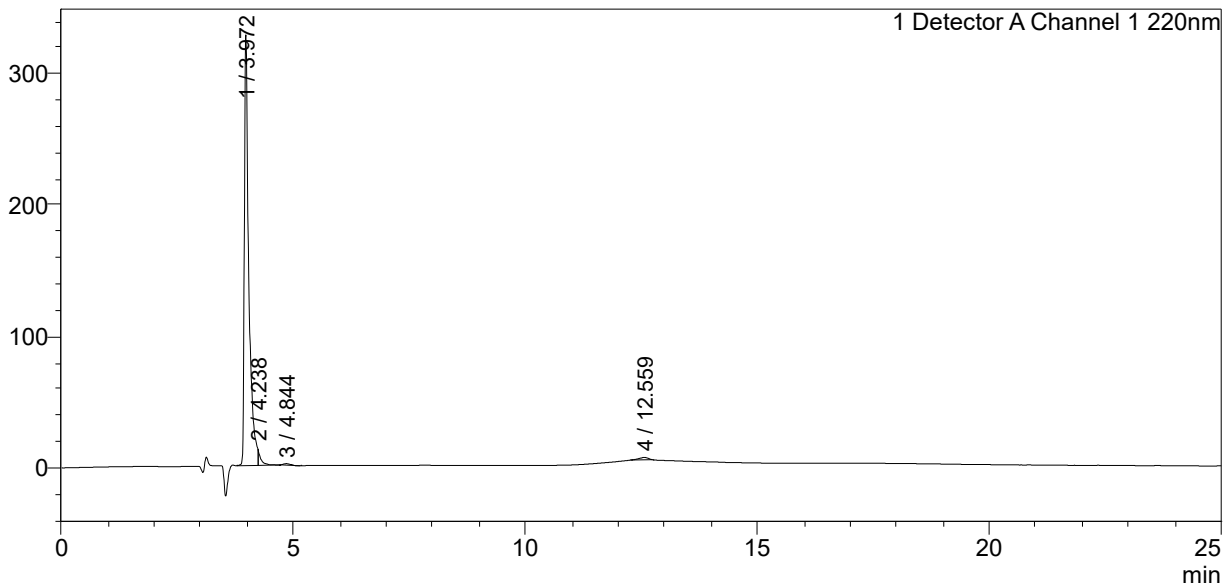

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	3.972	2194416	327941	96.011
2	4.238	53980	12016	2.362
3	4.844	11819	1174	0.517
4	12.559	25380	1822	1.110
Total		2285594	342953	100.000