

Sample Name : Arg-Gly-Asp-Cys
 Cat. No. : RP10860
 Lot. No. : E0661221E
 Time Processed : 17:11:40
 Month-Day-Year Processed : 05/30/2021


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

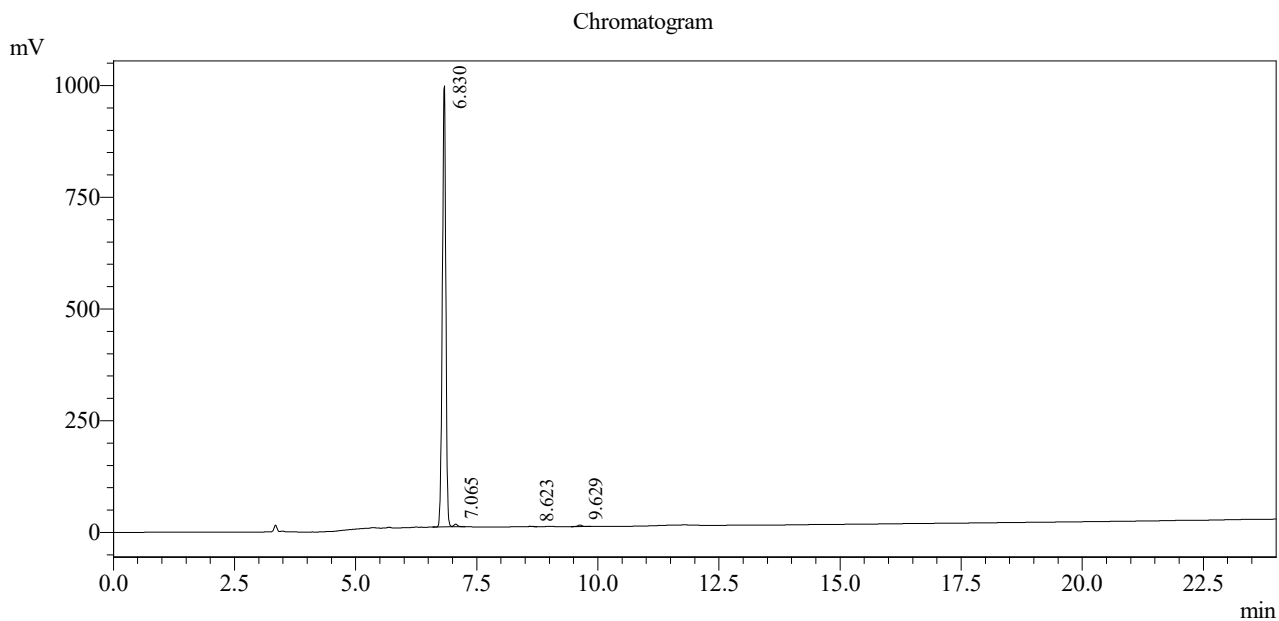

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	6.830	4967929	986860	98.975
2	7.065	31034	6026	0.618
3	8.623	1149	320	0.023
4	9.629	19252	3335	0.384
Total		5019364	996541	100.000