

Sample Name :NPF
 Cat No. : RP10470
 Lot No. :E4803119I
 Time Processed : 16:07:26
 Month-Day-Year Processed : 09/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

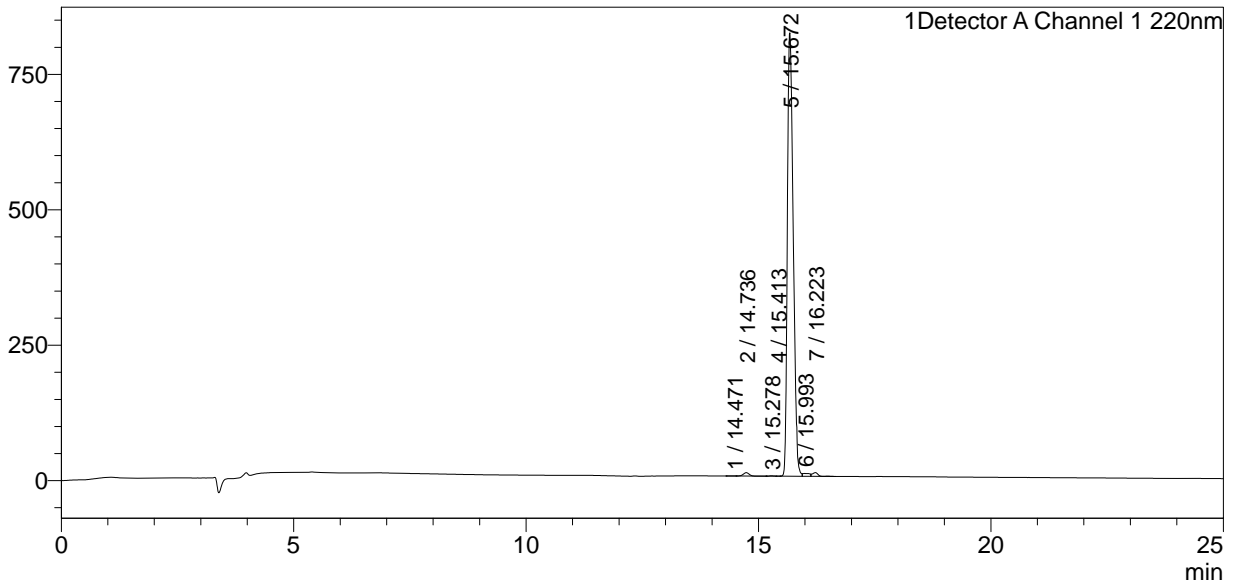

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.471	910	105	0.012
2	14.736	55575	6321	0.759
3	15.278	4447	708	0.061
4	15.413	1000	210	0.014
5	15.672	7144967	818539	97.608
6	15.993	53777	5180	0.735
7	16.223	59352	6864	0.811
Total		7320029	837928	100.000