

Sample Name :Gly-Phe-Arg
 Cat. No. : RP10590
 Lot. No. : PE5341903
 Time Processed : 12:54:20
 Month-Day-Year Processed : 03/22/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	10	
25.00	Pumps	Pump A B.Conc	70	
25.01	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	10	
40.00	Pumps	Pump A B.Conc	10	
40.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

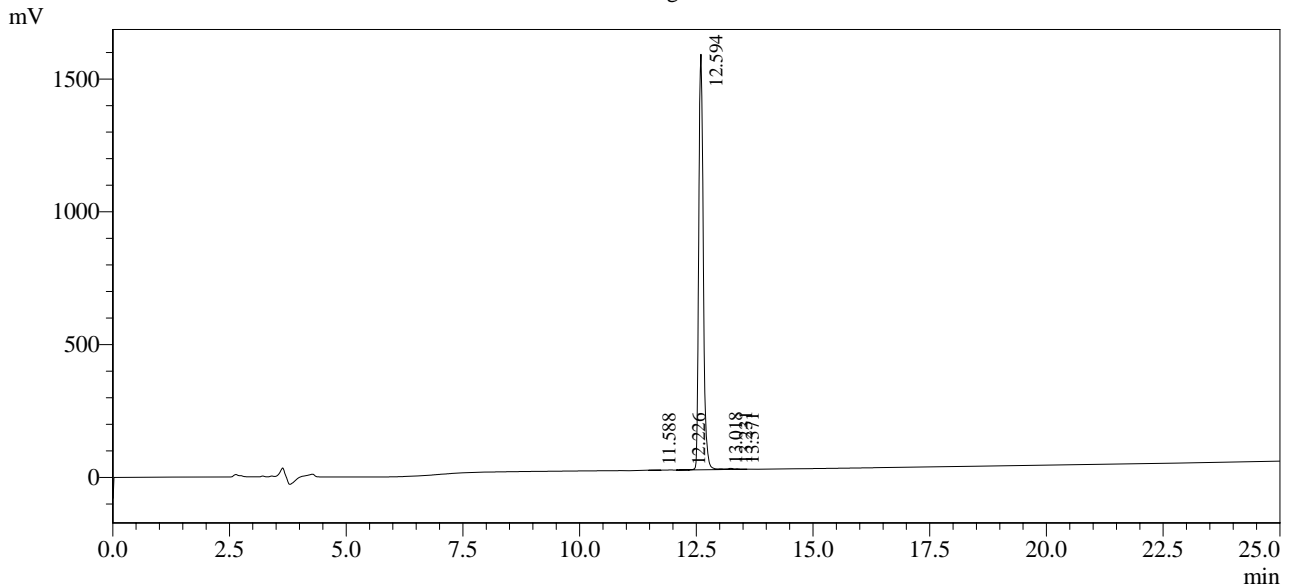

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.588	8584	1501	0.080
2	12.226	3528	408	0.033
3	12.594	10662712	1564413	99.252
4	13.018	24740	2939	0.230
5	13.231	31192	4049	0.290
6	13.371	12332	1983	0.115
Total		10743087	1575292	100.000