

Sample Name :Bradykinin (2-9)  
 Cat No. :RP11135  
 Lot No. :E7334619L  
 Time Processed :12:36:27  
 Month-Day-Year Processed :12/15/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ17010508

<Chromatogram>

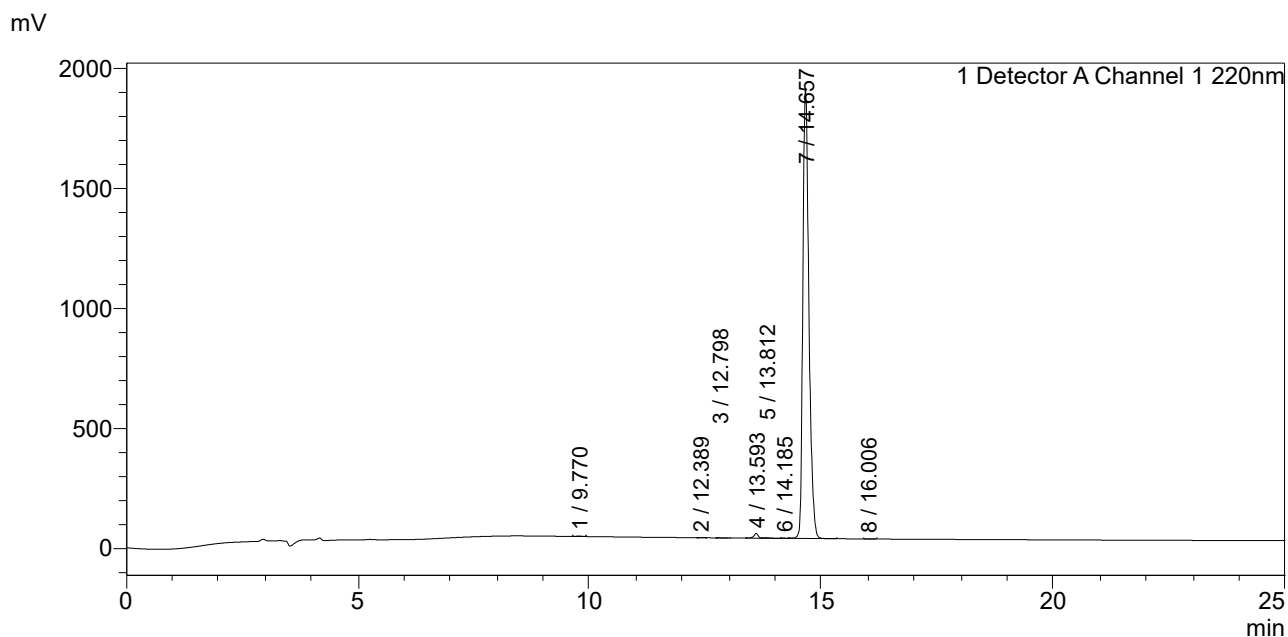

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.770	11661	1883	0.067
2	12.389	3018	481	0.017
3	12.798	2907	446	0.017
4	13.593	124626	19609	0.719
5	13.812	20307	2215	0.117
6	14.185	3382	751	0.020
7	14.657	17153919	1880597	99.026
8	16.006	2843	416	0.016
Total		17322663	1906397	100.000