

Sample Name :LAH4  
 Cat No. :RP20096  
 Lot No. : PE8771902  
 Time Processed : 23:27:10  
 Month-Day-Year Processed : 03/01/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment:GK12010012

### <Chromatogram>

mV

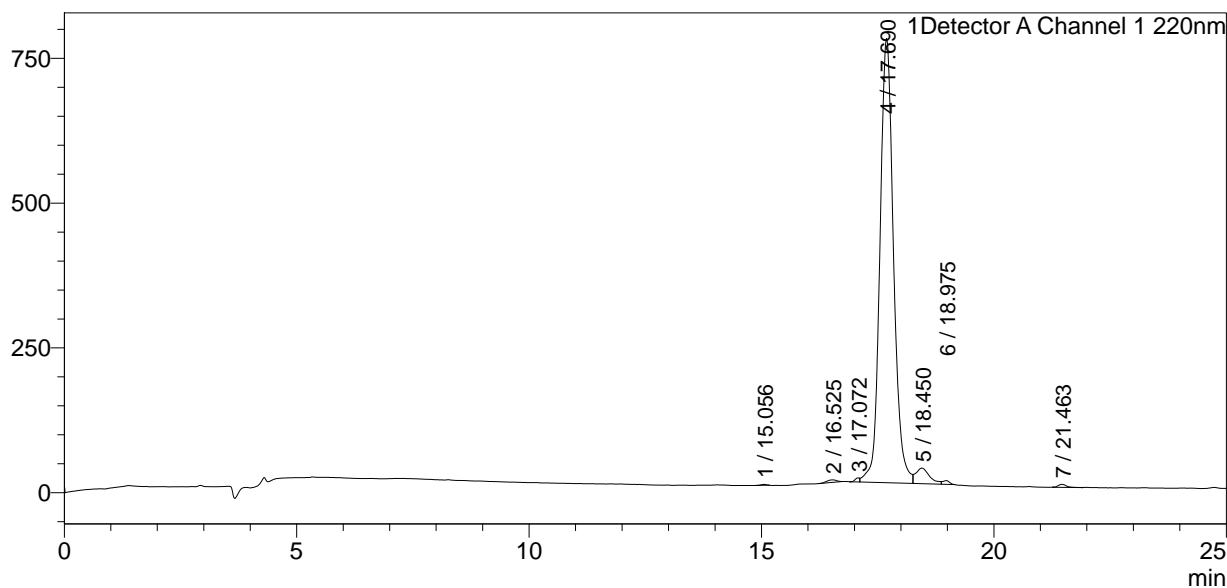

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.056	11120	1406	0.068
2	16.525	65339	4366	0.398
3	17.072	48127	6975	0.293
4	17.690	15607553	766858	95.119
5	18.450	551986	26859	3.364
6	18.975	63913	6378	0.390
7	21.463	60411	5106	0.368
Total		16408449	817947	100.000