

Sample Name : Endomorphin-2
 Cat. No. : RP10926
 Lot. No. : E4767519I
 Time Processed :21:46:52
 Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	30	
25.00	Pumps	Pump A B.Conc	90	
25.01	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	30	
40.00	Pumps	Pump A B.Conc	30	
40.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

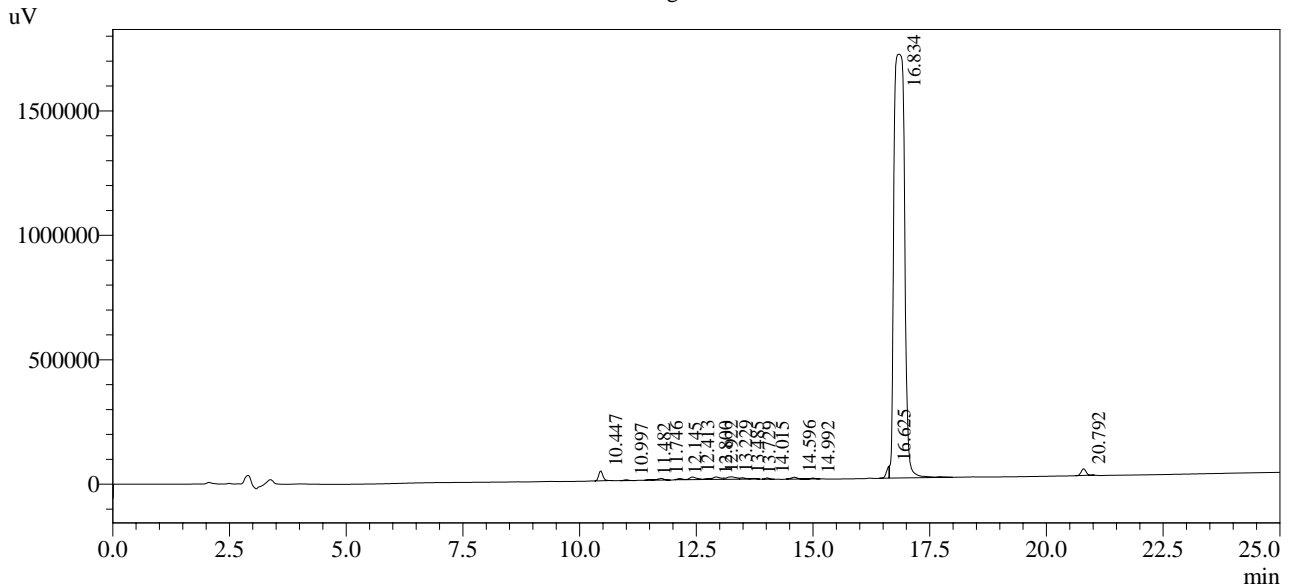

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.447	249448	39495	0.880
2	10.997	23803	3424	0.084
3	11.482	16580	2630	0.058
4	11.746	67560	6765	0.238
5	12.145	34892	4786	0.123
6	12.413	108248	10228	0.382
7	12.800	33345	3860	0.118
8	12.922	108978	9845	0.384
9	13.229	142205	9865	0.502
10	13.485	45251	5362	0.160
11	13.729	16893	2246	0.060
12	14.015	32097	5149	0.113
13	14.596	73443	7356	0.259
14	14.992	23732	3535	0.084
15	16.625	204015	47886	0.720
16	16.834	26975786	1702637	95.153
17	20.792	193711	26644	0.683
Total		28349987	1891714	100.000