

Sample Name : Syntide 2  
 Cat. No. : RP10322  
 Lot. No. : PE7071811  
 Time Processed : 8:53:57  
 Month-Day-Year Processed : 11/10/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

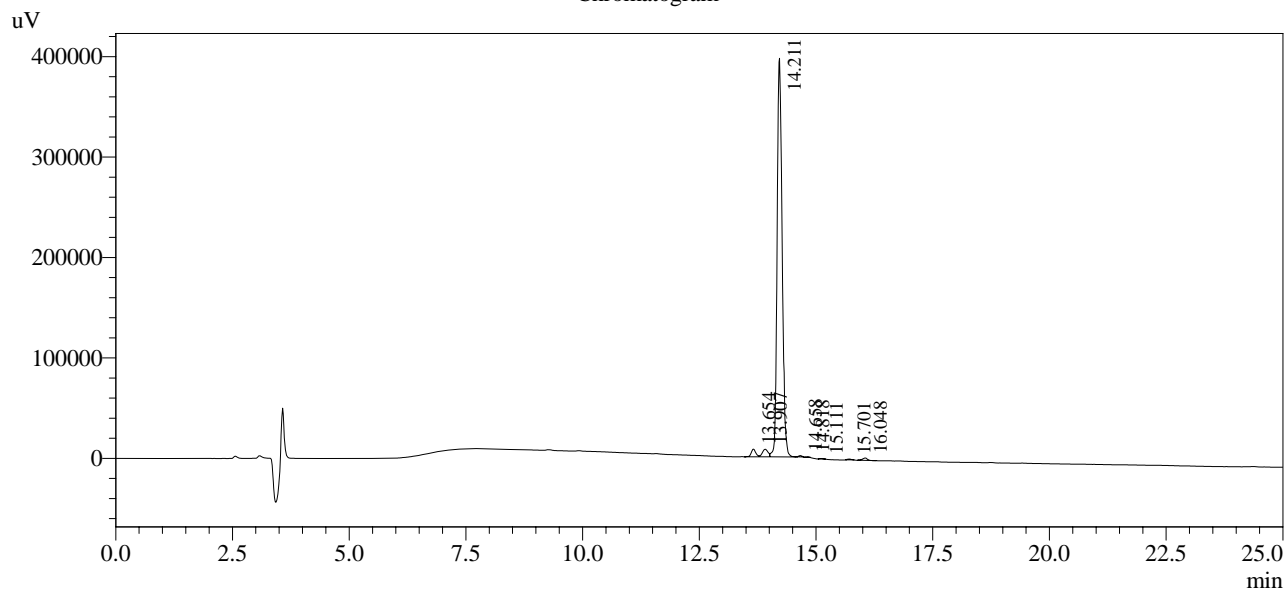

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.654	52873	7753	1.702
2	13.907	63409	7531	2.041
3	14.211	2959541	396895	95.248
4	14.658	6295	1291	0.203
5	14.818	1555	445	0.050
6	15.111	2267	453	0.073
7	15.701	4658	787	0.150
8	16.048	16612	2367	0.535
Total		3107208	417522	100.000