

Sample Name: β -Amyloid (13-27)
 Cat No. : RP20170
 Lot No. : E7037719J
 Time Processed: 12:09:22 AM
 Month-Day-Year Processed :10/02/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

mV

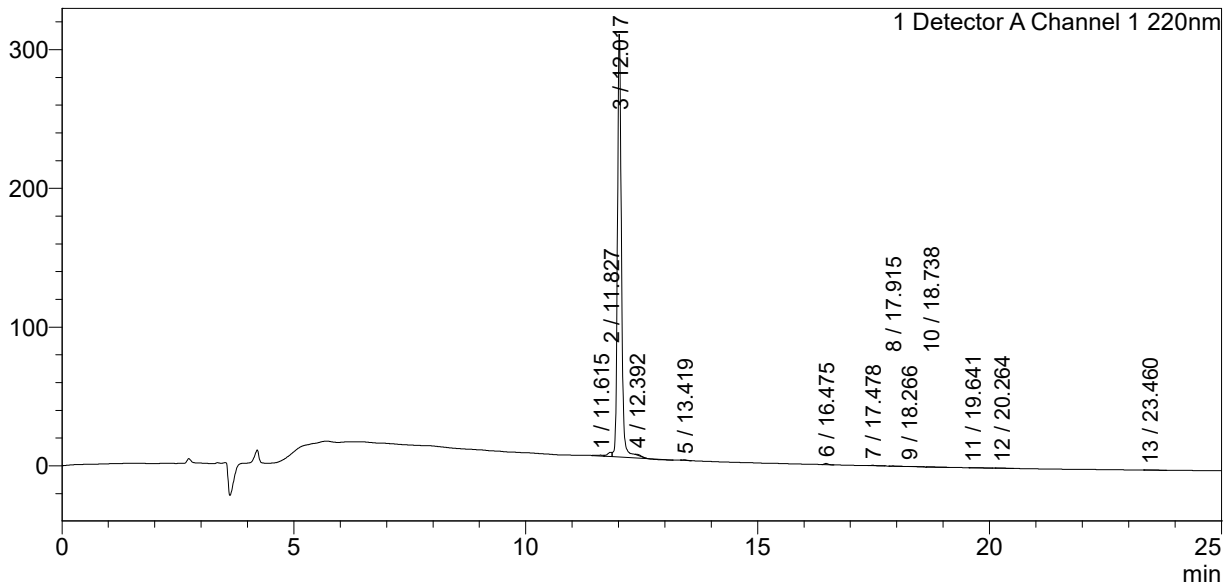

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.615	5991	600	0.321
2	11.827	19632	3051	1.052
3	12.017	1818982	304872	97.467
4	12.392	3202	430	0.172
5	13.419	2407	396	0.129
6	16.475	4687	877	0.251
7	17.478	2246	321	0.120
8	17.915	1189	94	0.064
9	18.266	1060	45	0.057
10	18.738	1889	127	0.101
11	19.641	1921	82	0.103
12	20.264	1920	184	0.103
13	23.460	1133	92	0.061
Total		1866259	311172	100.000