

Sample Name :CTTHWGFTLC, CYCLIC
 Cat No.: RP20386
 Lot No.: E6097920B
 Time Processed :9:29:54 AM
 Month-Day-Year Processed :02/08/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010325

<Chromatogram>

mV

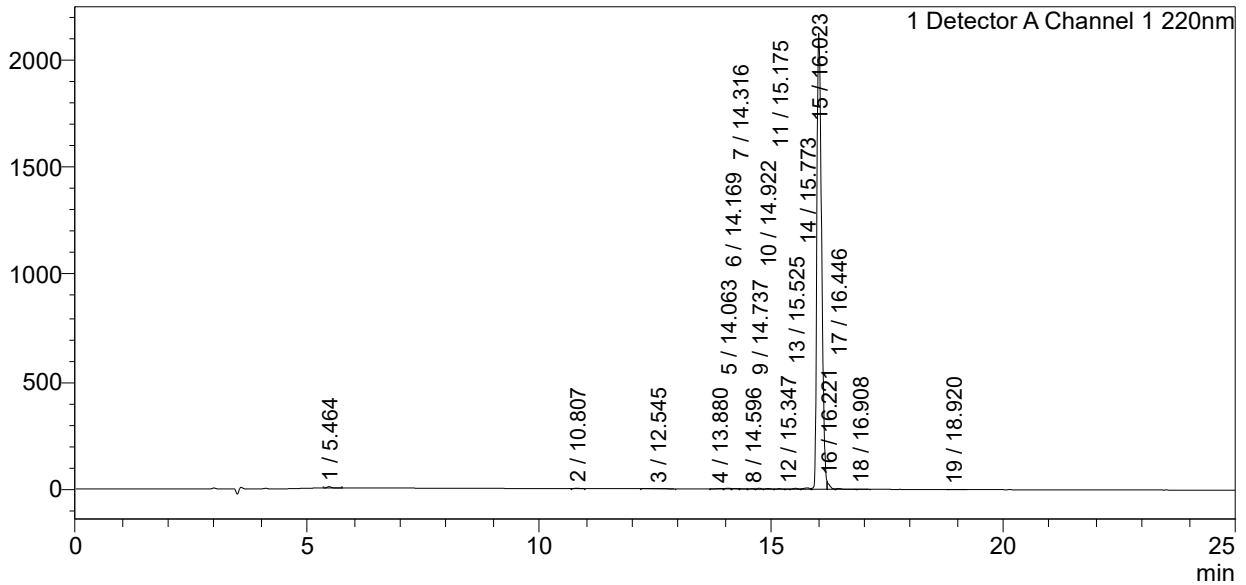

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.464	38332	6561	0.244
2	10.807	16621	2580	0.106
3	12.545	32563	1318	0.207
4	13.880	21210	2620	0.135
5	14.063	29883	3716	0.190
6	14.169	17905	2684	0.114
7	14.316	14638	1535	0.093
8	14.596	15525	2301	0.099
9	14.737	23789	3788	0.151
10	14.922	25498	3159	0.162
11	15.175	18629	1998	0.119
12	15.347	12272	1811	0.078
13	15.525	31367	3863	0.200
14	15.773	57378	6015	0.365
15	16.023	15221410	2128696	96.856

Peak#	Ret. Time	Area	Height	Area%
16	16.221	109115	28804	0.694
17	16.446	26376	3306	0.168
18	16.908	1203	151	0.008
19	18.920	1722	539	0.011
Total		15715437	2205447	100.000