

Sample Name : Myelin Basic Protein (MBP) (68-82), guinea pig  
 Cat. No. : RP10605  
 Lot. No. : E4090419H  
 Time Processed : 10:07:40 AM  
 Month-Day-Year Processed : 08/29/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

### <Chromatogram>

mV

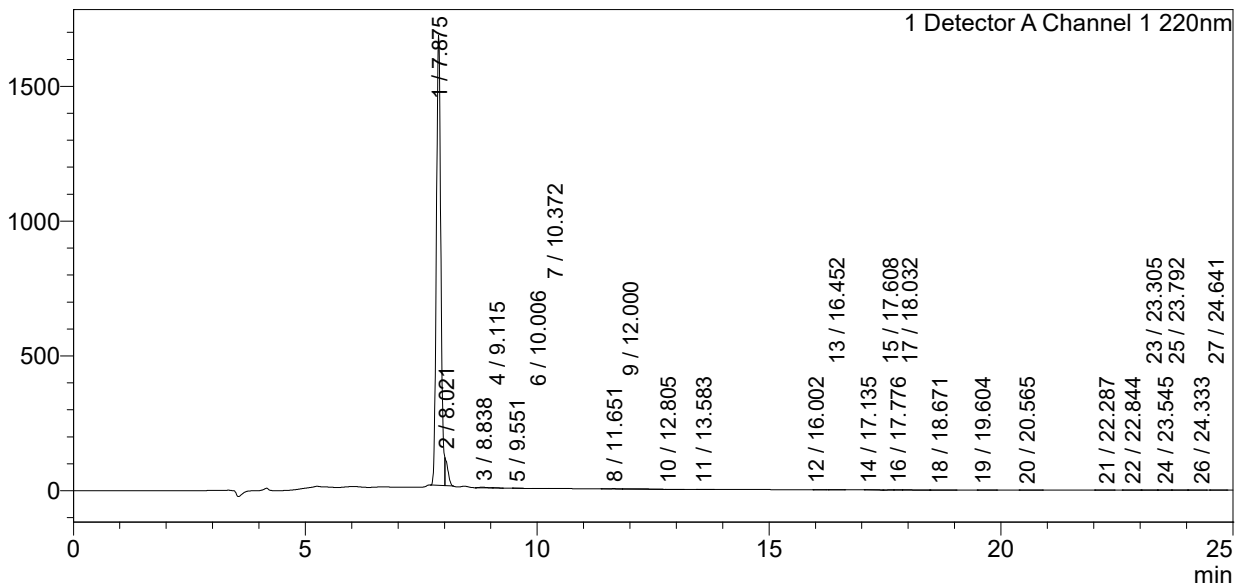

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.875	11196143	1669347	95.167
2	8.021	436110	99528	3.707
3	8.838	21505	1862	0.183
4	9.115	1888	301	0.016
5	9.551	3205	536	0.027
6	10.006	2101	237	0.018
7	10.372	3627	260	0.031
8	11.651	17728	1284	0.151
9	12.000	39192	1102	0.333
10	12.805	1232	46	0.010
11	13.583	3441	286	0.029
12	16.002	2003	191	0.017
13	16.452	1870	182	0.016
14	17.135	1579	99	0.013
15	17.608	1389	144	0.012

Peak#	Ret. Time	Area	Height	Area%
16	17.776	2176	200	0.018
17	18.032	4650	273	0.040
18	18.671	4138	200	0.035
19	19.604	1537	82	0.013
20	20.565	1599	93	0.014
21	22.287	1880	114	0.016
22	22.844	2453	175	0.021
23	23.305	1005	70	0.009
24	23.545	2904	229	0.025
25	23.792	2741	204	0.023
26	24.333	3799	241	0.032
27	24.641	2818	187	0.024
Total		11764712	1777471	100.000