

Sample Name :Melittin
 Cat No. :RP10290
 Lot No. :E5790420C
 Time Processed :8:13:39
 Month-Day-Year Processed :04/04/20

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

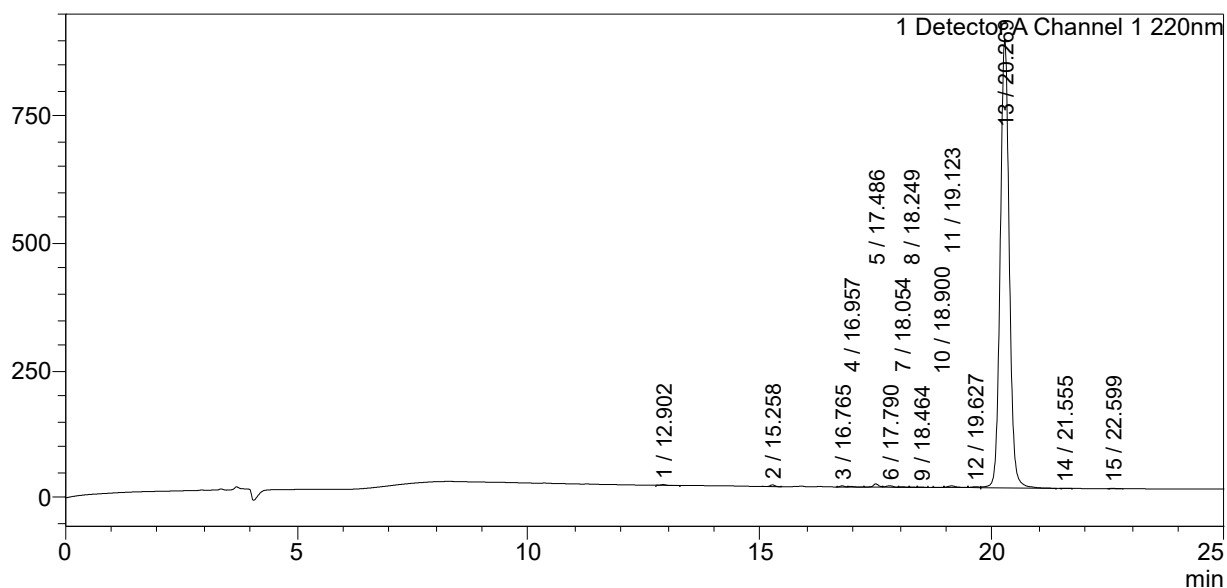

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.902	8792	1473	0.072
2	15.258	23168	3523	0.191
3	16.765	16735	2502	0.138
4	16.957	12177	1381	0.100
5	17.486	56588	6761	0.466
6	17.790	30751	2845	0.253
7	18.054	9225	1124	0.076
8	18.249	2012	359	0.017
9	18.464	3566	449	0.029
10	18.900	3940	537	0.032
11	19.123	41750	3264	0.344
12	19.627	19856	1717	0.164
13	20.269	11905250	880934	98.054
14	21.555	3335	439	0.027
15	22.599	4322	585	0.036

Peak#	Ret. Time	Area	Height	Area%
Total		12141466	907892	100.000