

Sample Name :Mastoparan
 Cat No.: RP10465
 Lot No.: E20407201
 Time Processed :12:56:05
 Month-Day-Year Processed :10/12/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

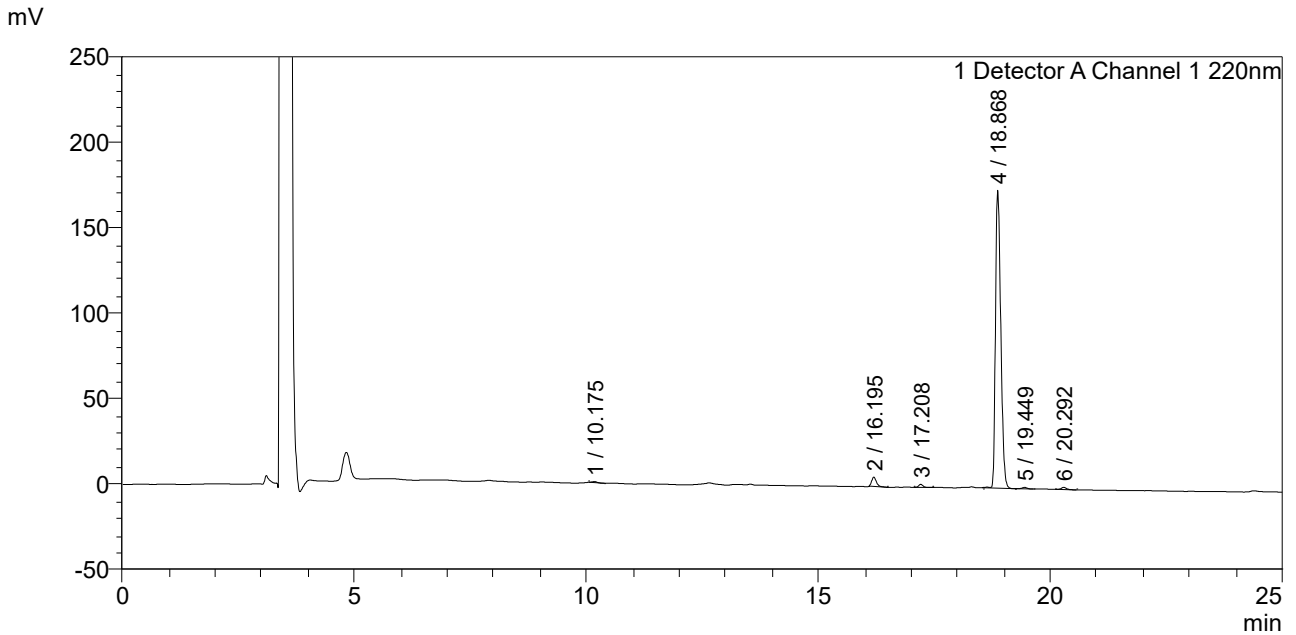

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.175	4053	634	0.280
2	16.195	37080	5344	2.561
3	17.208	10427	1723	0.720
4	18.868	1379365	174305	95.269
5	19.449	7158	899	0.494
6	20.292	9787	1303	0.676
Total		1447869	184209	100.000