


Mass Spectrum

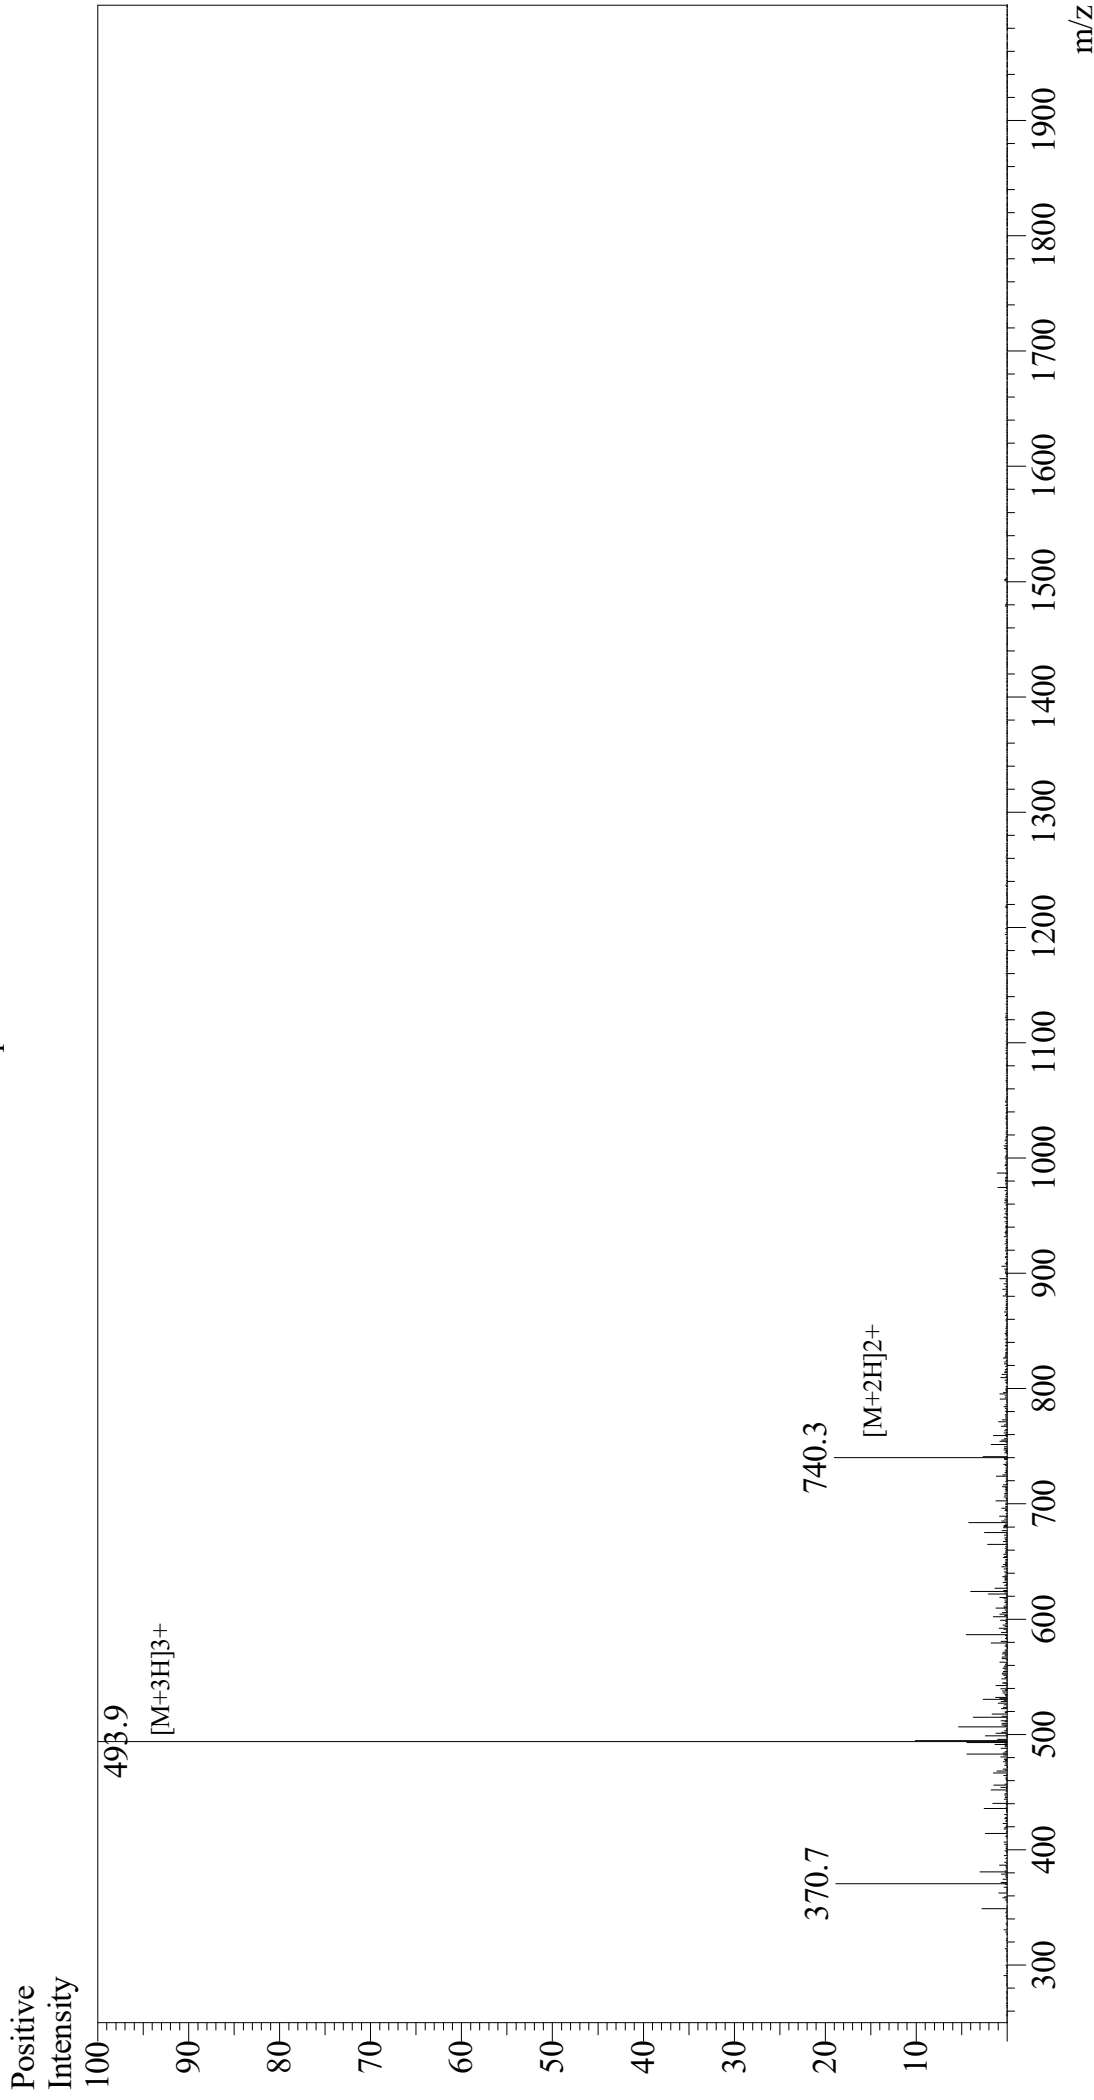

Sample Information

Month-Day Processed : 10/12/20
Time Processed : 11:24:03 AM
Injection Volume : 0.3
Sample Name : Mastoparan
Cat No. : RP10465
Lot No. : E2040720I
Theoretical MW : 1478.80
Observed MW : 1478.7

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH