

Sample Name : NP (396-404)
 Cat. No. : RP20090
 Lot. No. : E9143819L
 Time Processed : 7:50:12
 Month-Day-Year Processed : 12/22/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

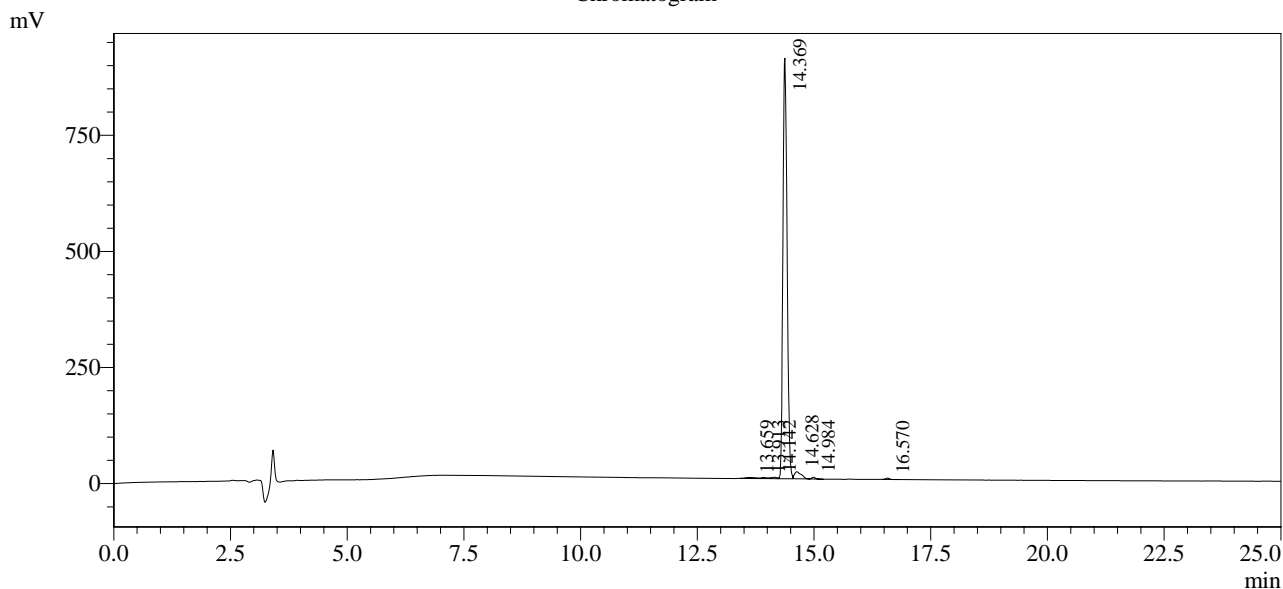

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.659	32945	2253	0.555
2	13.913	17727	2506	0.299
3	14.142	30513	2956	0.514
4	14.369	5660799	905517	95.406
5	14.628	155133	15151	2.615
6	14.984	20303	3741	0.342
7	16.570	15933	2903	0.269
Total		5933354	935027	100.000