

Sample Name : Glucagon (1-29), Human  
 Cat No.: RP10772  
 Lot No.: E3611419K  
 Time Processed : 20:51:12  
 Month-Day-Year Processed : 11/15/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm  
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
45.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010324

### <Chromatogram>

mV

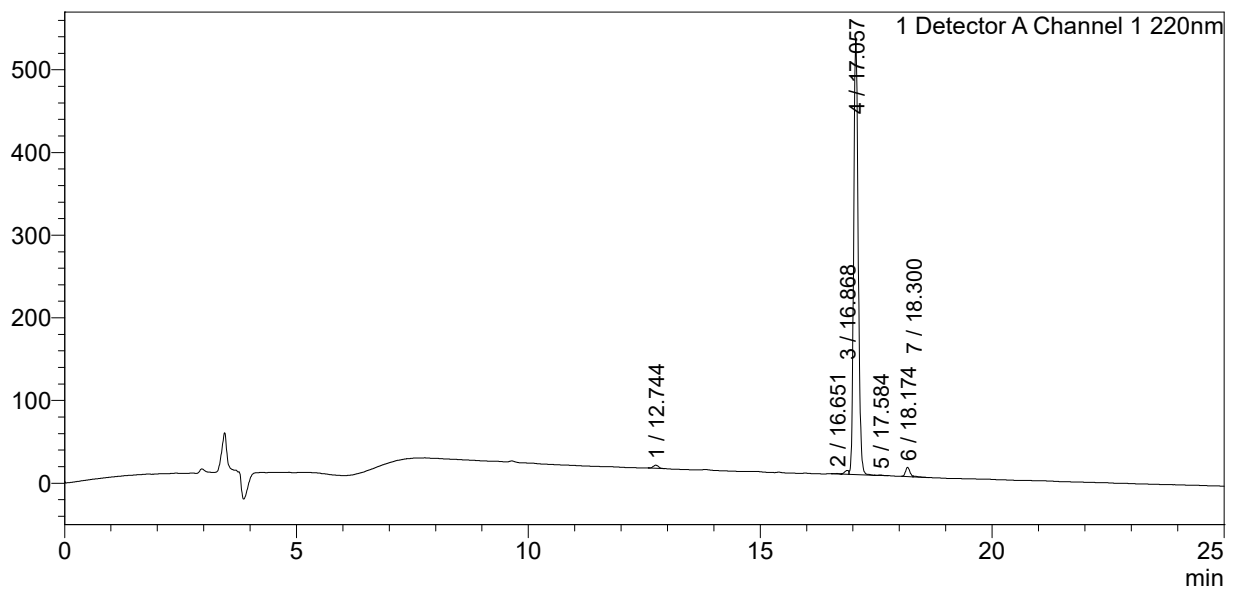

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.744	28210	3725	0.759
2	16.651	4221	600	0.114
3	16.868	30095	4809	0.810
4	17.057	3570357	528400	96.050
5	17.584	3357	490	0.090
6	18.174	72514	11203	1.951
7	18.300	8438	1069	0.227
Total		3717193	550295	100.000