

Sample Name :Peptide YY (PYY), human
 Cat No. :RP10355
 Lot No. :PE2011905
 Time Processed :9:19:56
 Month-Day-Year Processed :06/02/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

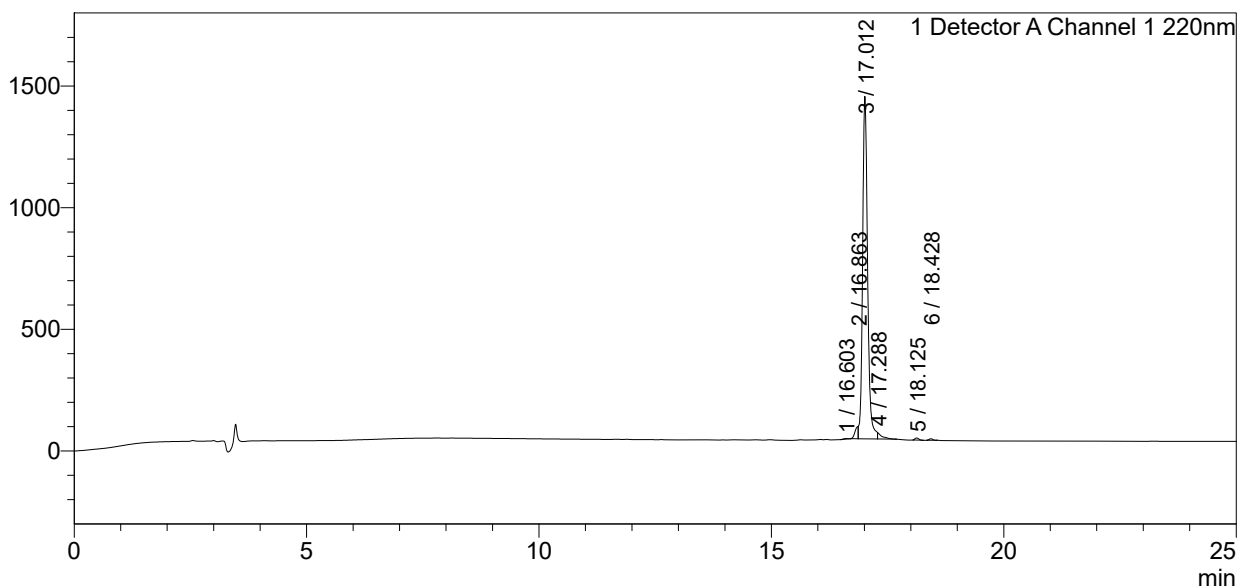

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.603	16727	2423	0.151
2	16.863	241303	50015	2.184
3	17.012	10542718	1407456	95.440
4	17.288	164706	27050	1.491
5	18.125	46496	8612	0.421
6	18.428	34542	6399	0.313
Total		11046492	1501955	100.000